

Nota de aplicación

## Hydroxyisophthalic Acid

---

Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.

---


### Abstract

This application brief highlights the analysis of hydroxyisophthalic acid using XTerra Columns.

---

## Introduction

The compound analyzed in this study is hydroxyisophthalic acid.

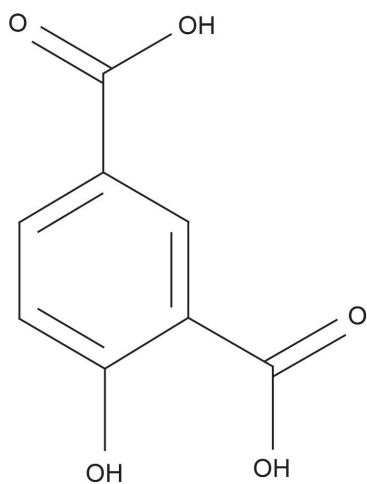

## Hydroxyisophthalic acid

---

## Experimental


### Conditions

Column:	XTerra RP <sub>18</sub> 4.6 x 150 mm, 5 μm
Part number:	186000492
Mobile phase:	pH 3.0: H <sub>2</sub> O/ACN/100 mM NH <sub>4</sub> COOH, pH 3.0 60:30:10 pH 7.0: H <sub>2</sub> O/ACN/100 mM NH <sub>4</sub> HCO <sub>3</sub> , pH 7.0 90:0:10

	pH 10.0 H <sub>2</sub> O/ACN/100 mM NH <sub>4</sub> HCO <sub>3</sub> , pH 10.0 90:0:10
Flow rate:	1.0 mL/min
Injection volume:	5 µL of 250 µg/mL
Temperature:	30 °C
Detection:	UV @ 260 nm
Instrument:	Alliance 2695, 2996 PDA
Mobile Phase pH	USP Tailing
3.0	1.17
7.0	1.23
10.0	1.23

---

## Results and Discussion

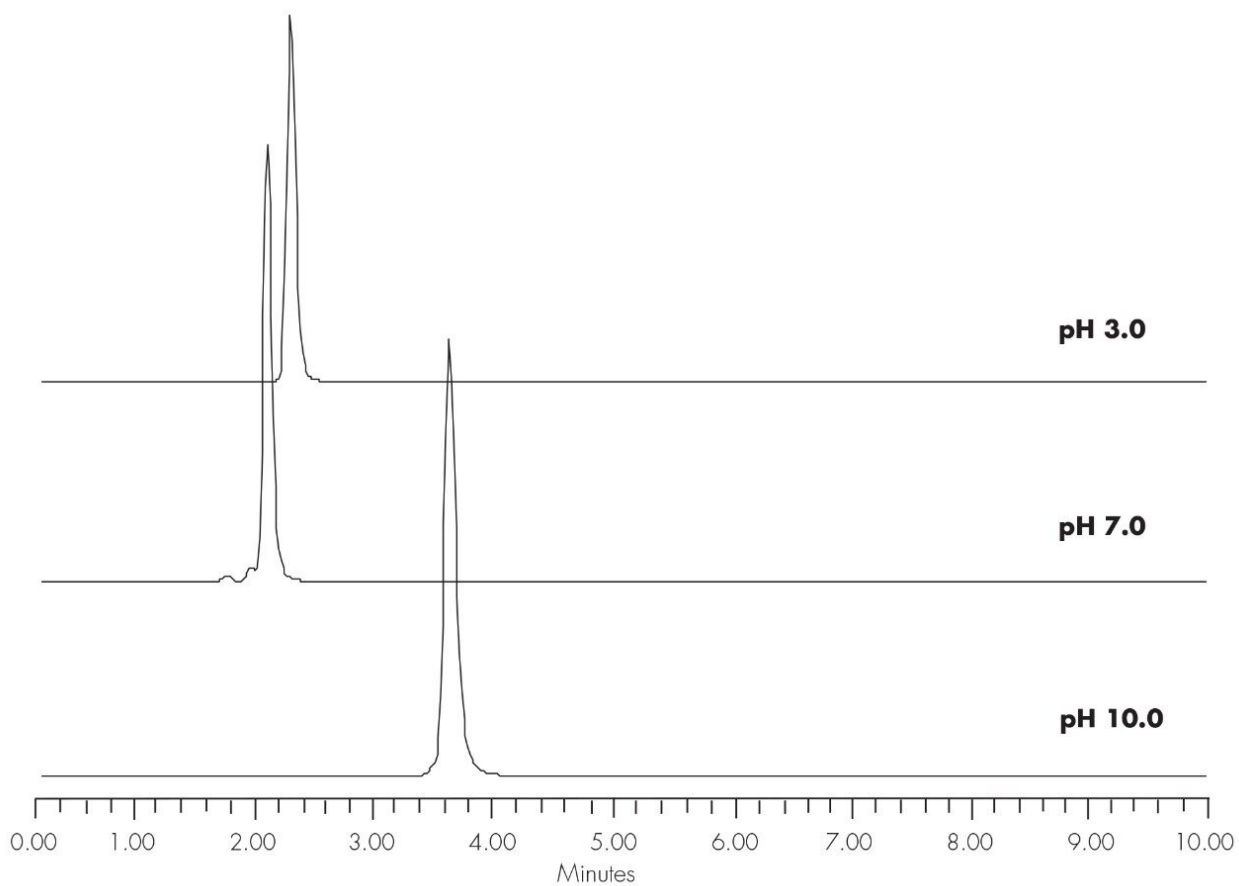

---

## Featured Products

Alliance HPLC System <<https://www.waters.com/534293>>

2998 Photodiode Array (PDA) Detector <<https://www.waters.com/1001362>>

WA20738.061, June 2002

© 2021 Waters Corporation. All Rights Reserved.