


Methylnicotinic Acid

Waters Corporation

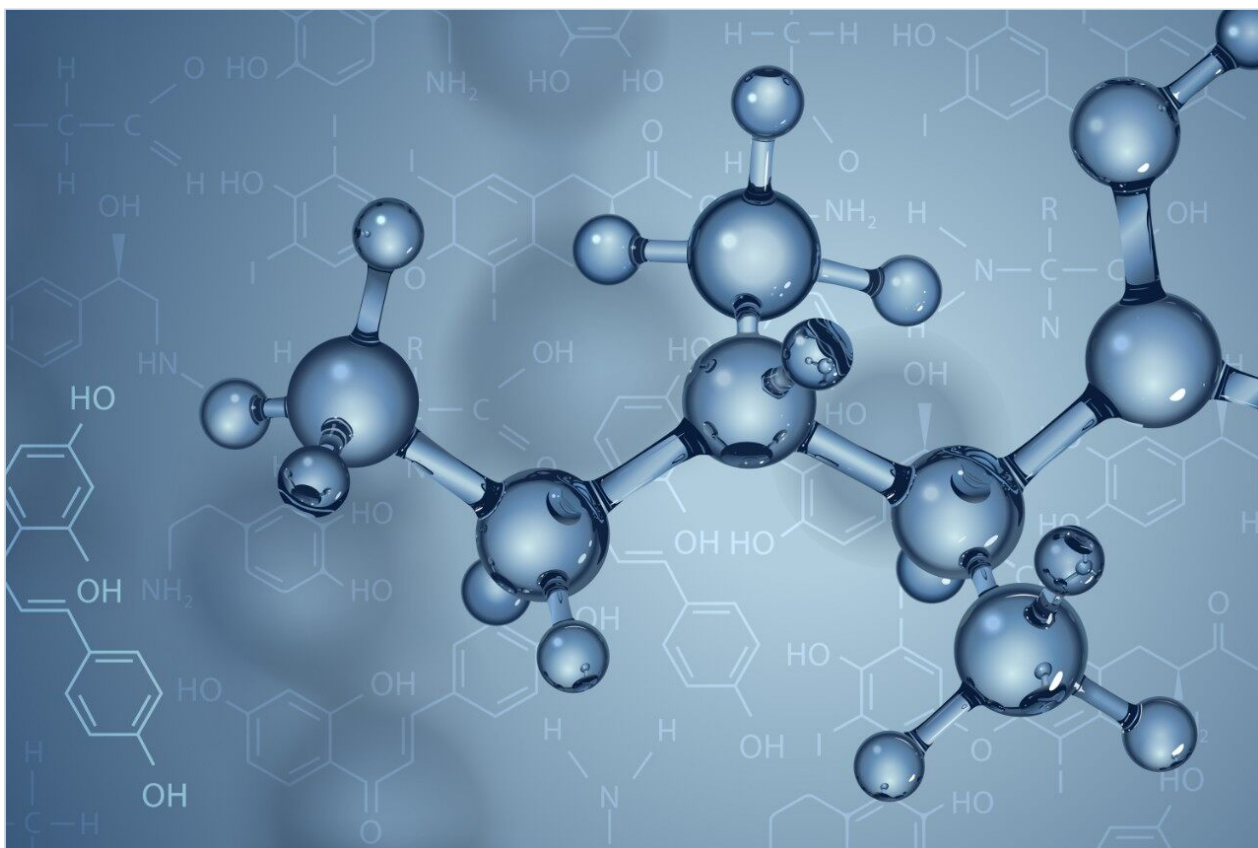


This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief highlights the analysis of methylnicotinic acid using XTerra Columns.

Introduction

The compound analyzed in this study is methylnicotinic acid.

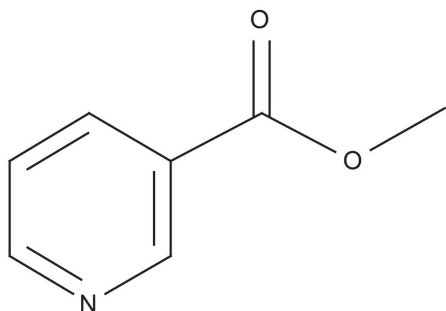

Methylnicotinic acid

Experimental


Conditions

| | |
|---------------|--|
| Column: | XTerra RP ₁₈ 4.6 x 150 mm, 5 μm |
| Part number: | 186000492 |
| Mobile phase: | pH 3.0: H ₂ O/ACN/100 mM NH ₄ COOH, pH 3.0 85:05:10 pH 7.0: H ₂ O/ACN/100 mM NH ₄ HCO ₃ , pH 7.0 85:05:10 pH 10.0 H ₂ O/ACN/100 mM NH ₄ HCO ₃ , pH 10.0 90:0:10 |
| Flow rate: | 1.0 mL/min |

Injection volume: 5 μ L of 250 μ g/mL
Temperature: 30 $^{\circ}$ C
Detection: UV @ 254 nm
Instrument: Alliance 2695, 2996 PDA

| Mobile Phase pH | USP Tailing |
|-----------------|-------------|
| 3.0 | 1.23 |
| 7.0 | 1.25 |
| 10.0 | 1.51 |

Results and Discussion

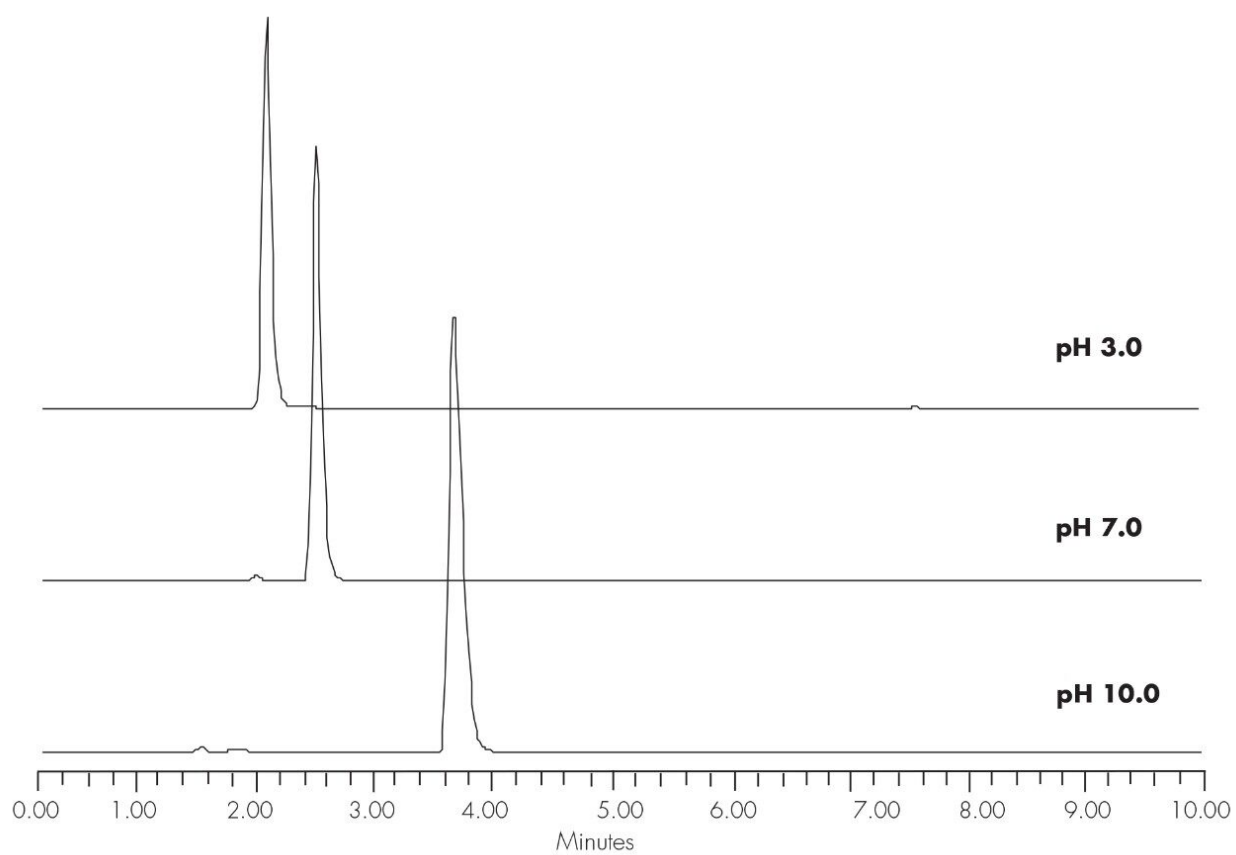

Featured Products

Alliance HPLC System <<https://www.waters.com/534293>>

2998 Photodiode Array (PDA) Detector <<https://www.waters.com/1001362>>

WA20738.070, June 2002

© 2021 Waters Corporation. All Rights Reserved.