

## Polar and Non-Polar Compounds Test Mix

---

Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.

---


### Abstract

This application brief highlights the analysis of polar and non-polar compounds test mix using XTerra C<sub>18</sub> columns.


---

## Introduction


Polar and non-polar compounds are analyzed in this application brief.



2-Amino-7-chloro-5-oxo-5H-[1,2,3-b]pyridine-3-carbonitrile



Acetanilide




6-Methyl-17-hydroxyprogesterone



3-Aminofluoranthene




Perylene




Triamcinolone



Naphtho(2,3-a)pyrene



Hydrocortisone



2-Bromofluorene

---

## Experimental

### Conditions

Column:

XTerra MS C<sub>18</sub> 4.6 x 20 mm, 3.5 μm (p/n: 186001891)

Mobile phase A:

0.1% HCOOH in H<sub>2</sub>O

Mobile phase B: 0.1% HCOOH in ACN

Flow rate: 3.0 mL/min

Injection volume: 10  $\mu$ L

Sample Concentration: 10  $\mu$ g/mL

Temperature: 30°C

Detection: UV @ 254 nm


Instrument: Alliance HT 2795, 2996 PDA

### Gradient

Time (min)	Profile	
	%A	%B
0.0	100	0
4.0	0	100

---

### Results and Discussion

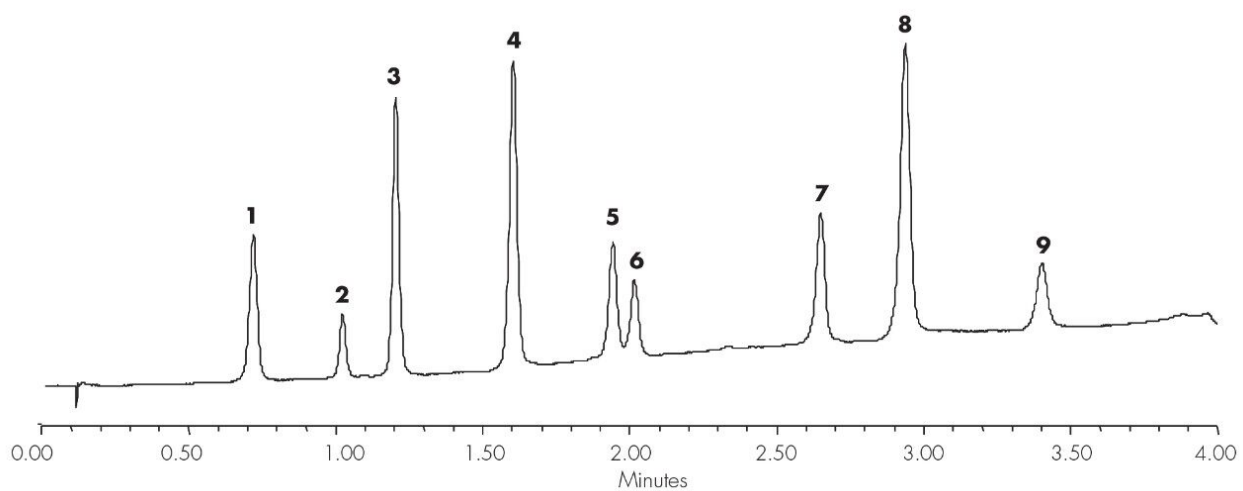

---

## Featured Products

Alliance HPLC <<https://www.waters.com/514248>>

WA20738.089, June 2002