

Dibucaine - LC/UV

Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief highlights the analysis of dibucaine using XTerra RP₁₈ columns.

Detection:


UV @ 280 nm

Instrument:

Alliance 2695, 2996 PDA

Mobile phase pH	USP Trailing
3	1.23
7	1.19
10	1.18

Results and Discussion

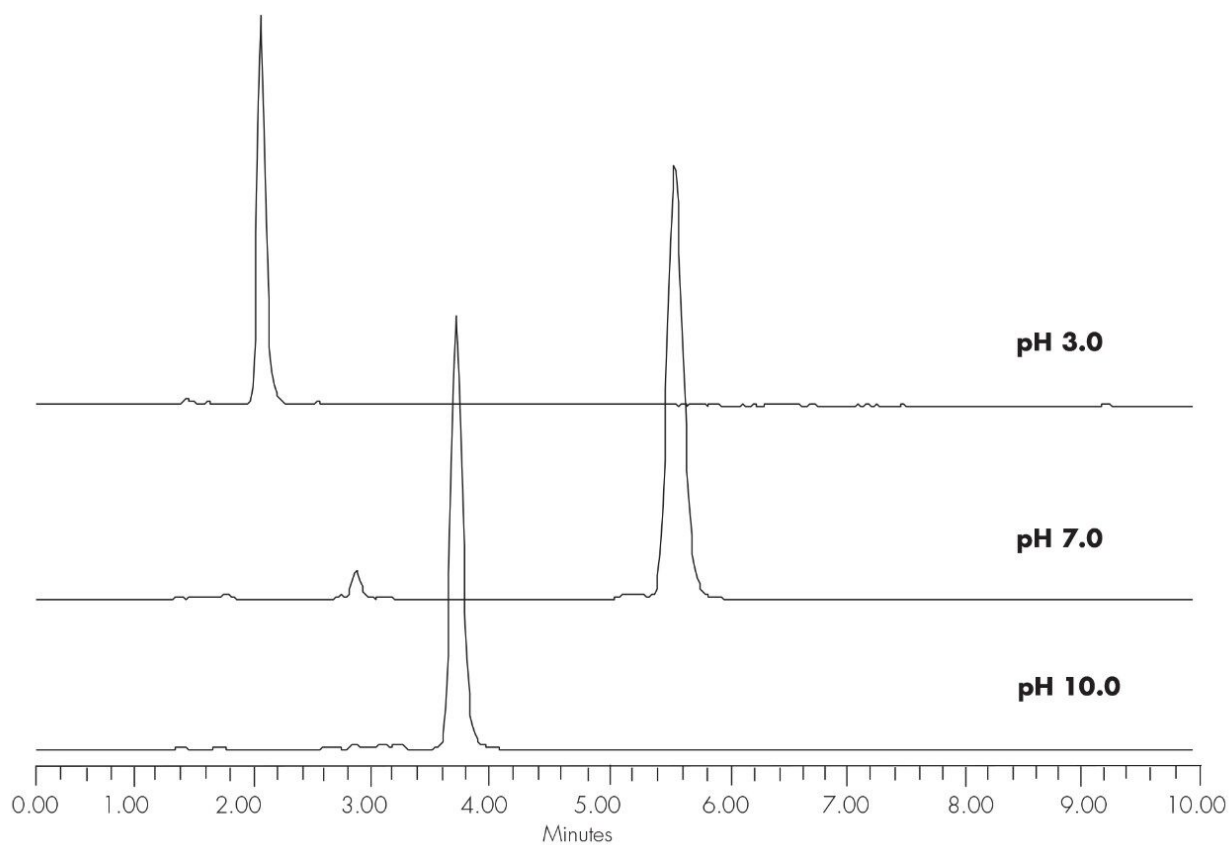

Featured Products

Alliance HPLC <<https://www.waters.com/514248>>

WA20738.034, June 2002

© 2021 Waters Corporation. All Rights Reserved.