

Applikationsbericht

Disopyramide

Waters Corporation


This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief demonstrates the analysis of disopyramide using Symmetry Columns.

Introduction

The compound analyzed in this study is Disopyramide.

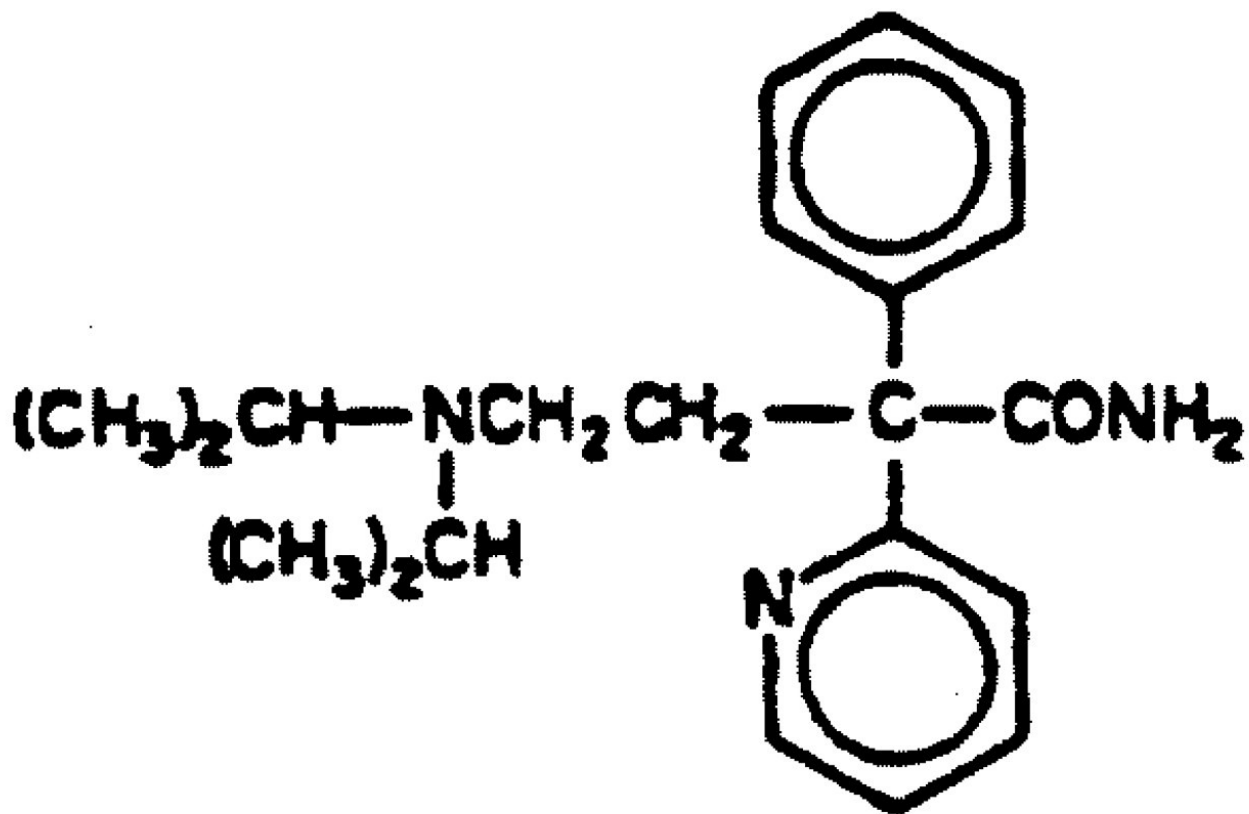

1. Disopyramide

Experimental

HPLC Method

Column:

Symmetry C₁₈, 3.9 x 150 mm, 5 μm

Part number:


WAT046980

Mobile phase:	50 mM potassium phosphate, pH 7.0/acetonitrile 70:30
Flow rate:	1.0 mL/min
Injection volume:	20 µL of 100 µg/mL sample
Detection:	UV @ 254 nm

USP Tailing Factors

1. 1.3

Results and Discussion

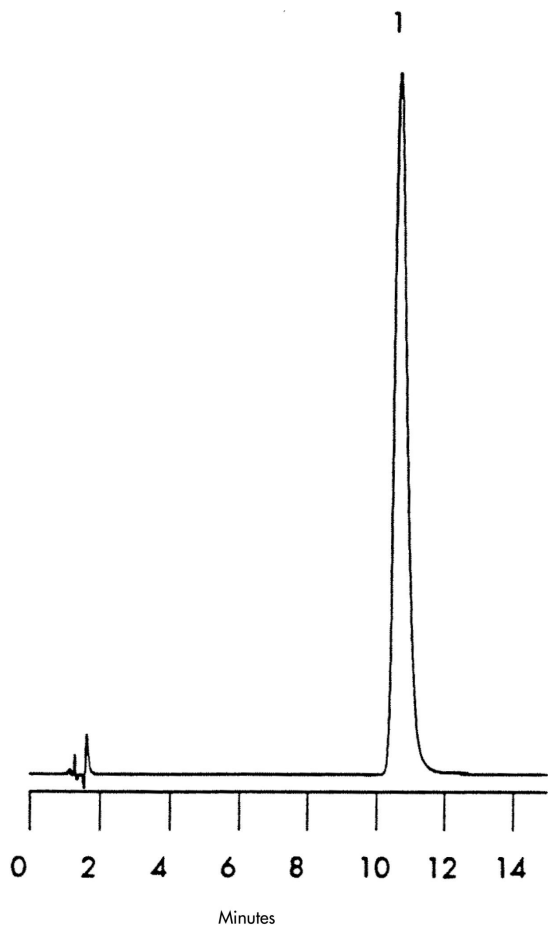

Featured Products

WA31763.78, June 2003

© 2022 Waters Corporation. All Rights Reserved.