

Application Note

## Disopyramide

---

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

---


### Abstract

This application brief demonstrates the analysis of disopyramide using Symmetry Columns.

---

### Introduction

The compound analyzed in this study is Disopyramide.

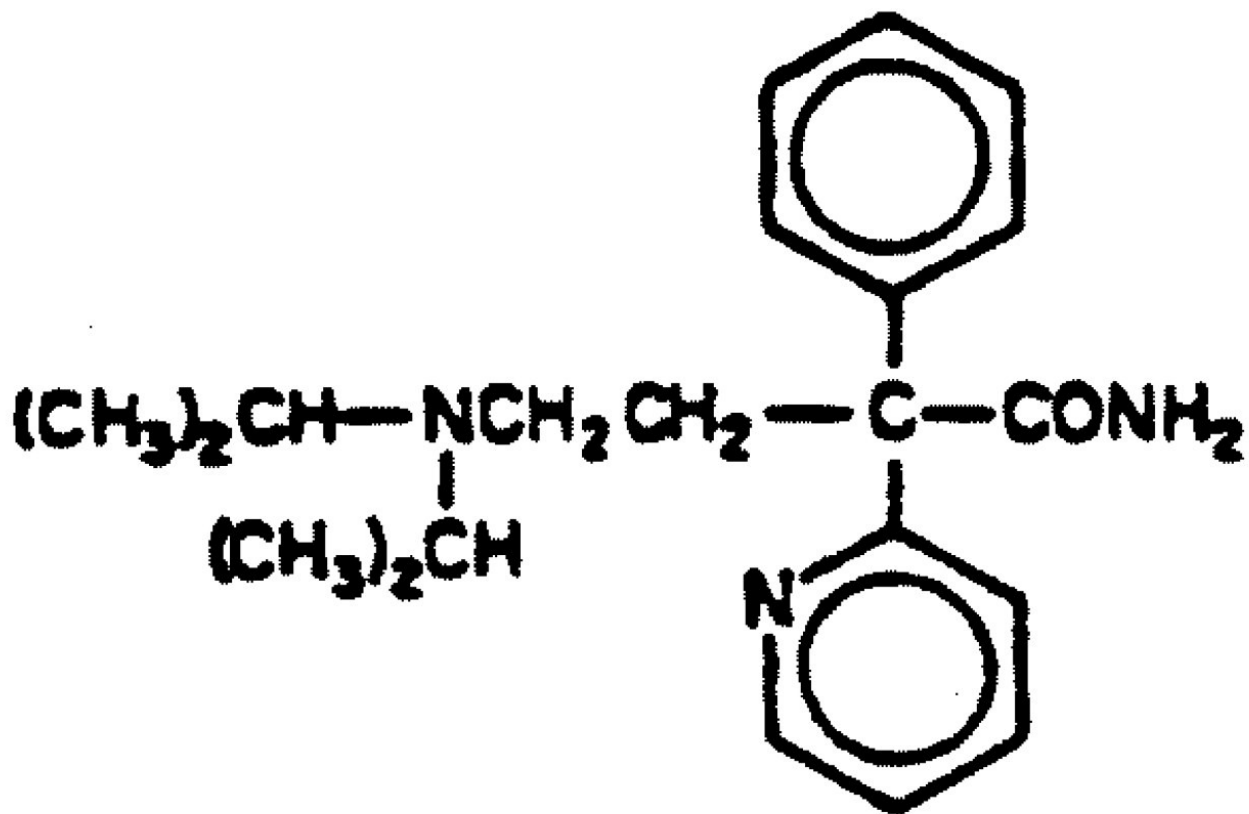

# 1. Disopyramide

---

Experimental

HPLC Method

Column:

Symmetry C<sub>18</sub>, 3.9 x 150 mm, 5 μm

Part number:

WAT046980


Mobile phase:	50 mM potassium phosphate, pH 7.0/acetonitrile 70:30
Flow rate:	1.0 mL/min
Injection volume:	20 $\mu$ L of 100 $\mu$ g/mL sample
Detection:	UV @ 254 nm

## USP Tailing Factors

1. 1.3

---

## Results and Discussion

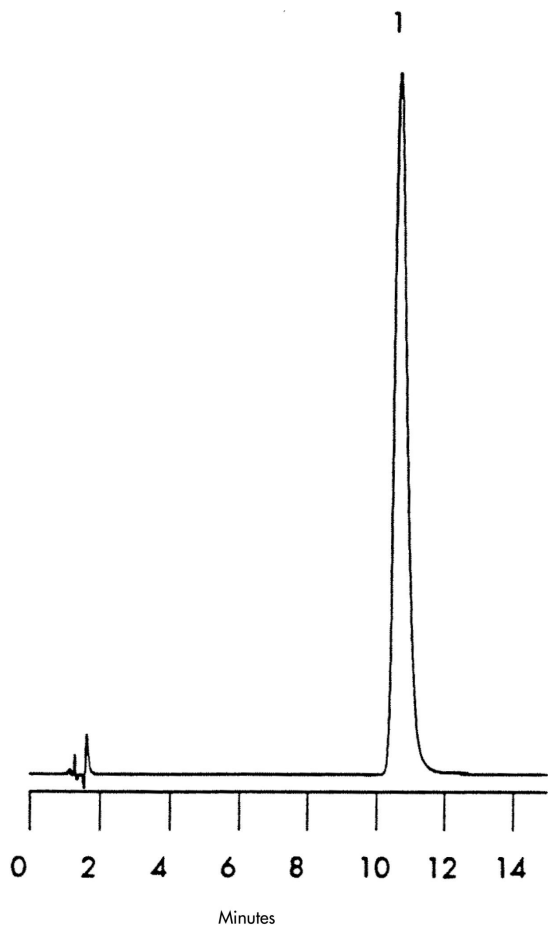

---

## Featured Products

WA31763.78, June 2003

© 2022 Waters Corporation. All Rights Reserved.