# Waters™



# Disopyramide

**Waters Corporation** 


This is an Application Brief and does not contain a detailed Experimental section.

#### **Abstract**

This application brief demonstrates the analysis of disopyramide using Symmetry Columns.

#### Introduction

The compound analyzed in this study is Disopyramide.

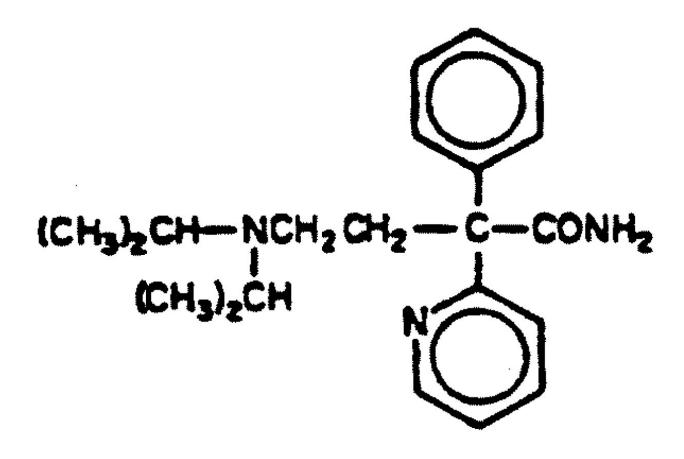

# 1. Disopyramide

## Experimental

#### **HPLC** Method

Column: Symmetry  $C_{18}$ ,  $3.9 \times 150$  mm,  $5 \mu m$ 

Part number: WAT046980

Mobile phase: 50 mM potassium phosphate, pH 7.0/acetonitrile

70:30

Flow rate: 1.0 mL/min


Injection volume: 20  $\mu$ L of 100  $\mu$ g/mL sample

Detection: UV @ 254 nm

### **USP Tailing Factors**

1. 1.3

### **Results and Discussion**

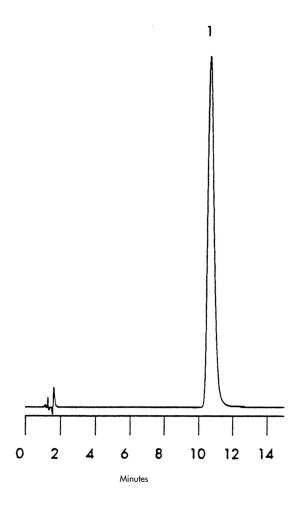

## **Featured Products**

WA31763.78, June 2003

© 2022 Waters Corporation. All Rights Reserved.