
Waters™

Applikationsbericht

Phenone Mixture

Waters Corporation

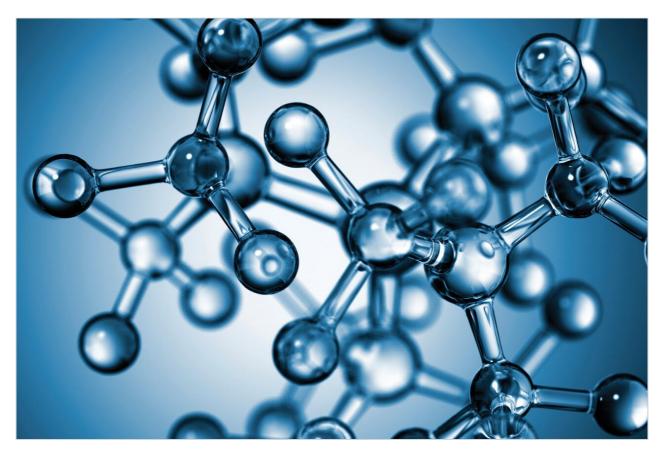

This is an Application Brief and does not contain a detailed Experimental section.


Abstract

This application brief demonstrates analysis of phenone mixture using Sunfire C_8 and C_{18} Columns.

Introduction

The compounds analysed in this study using Sunfire C_{18} Columns are -

Compounds	USP tailing	
1. Theophylline	1.31	
2. 2-Acetylfuran	1.15	
3. Acetanilide	1.16	
4. Acetophenone	1.18	
5. Propiophenone	1.14	
6. Butyrophenone	1.13	
7. Benzophenone	1.13	
8. Valerophenone	1.15	
9. Hexanophenone	1.06	
10. Heptanophenone 1.10		
11. Octanophenone	1.06	

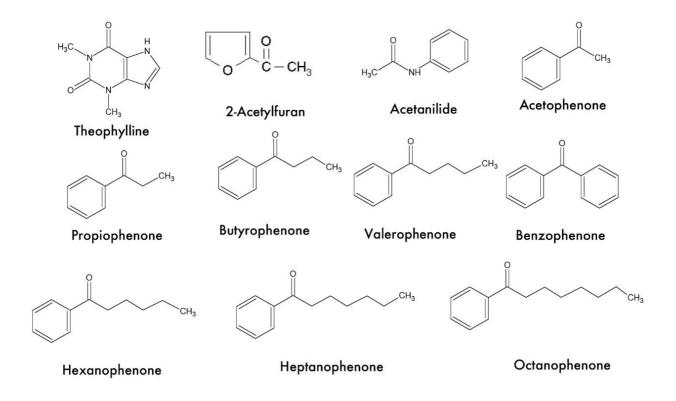


II compound mixture of phenones separated in under 4 minutes with SunFire C_{18} IS Column.

The compounds analysed in this study using Sunfire $\ensuremath{C_8}$ Columns are -

Compounds	USP tailing	
1. Theophylline	1.17	
2. 2-Acetylfuran	1.06	
3. Acetanilide	1.07	
4. Acetophenone	1.02	
5. Propiophenone*	1.00	
6. Butyrophenone*	0.87	
7. Benzophenone*	0.99	
8. Valerophenone*	1.02	
9. Hexanophenone* 0.99		
10. Heptanophenone*	one* 0.93	
11. Octanophenone*	1.03	

^{*}stock solution prepared in acetontrile

^{*:} stock solution prepared in acetontrile

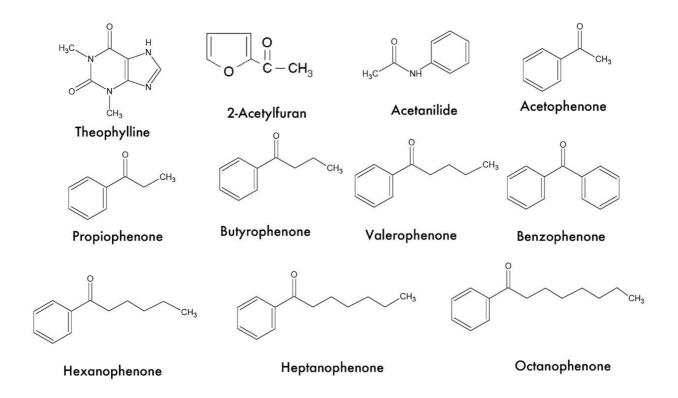

II compound mixture of phenones separated in under 4 minutes with SunFire C_8 IS Column.

Experimental

Conditions

Column: SunFire C_{18} 4.6 x 20 mm /S, 3.5 μ m

Part number: 186002549

Mobile phase A: 0.1% HCOOH in Water

Mobile phase B: 0.1% HCOOH in ACN

Flow rate: 3.0 mL/min

Injection vo	lumai	10 ו	
injection vc	nume.	10	ᆈᆫ

Sample concentration: 10 μ g/mL in water

Temperature: 30 °C

Detection: UV @ 254 nm

Instrument: Alliance 2695 with 2996 PDA

Gradient

Time	Prof	file
(min)	%A	%B
0.0	100	0
4.0	0	100

Conditions

Column: SunFire C_8 4.6 x 20 mm /S, 3.5 μ m

Part number: 186002699

Mobile phase A: Water

Mobile phase B: Acetonitrile

Mobile phase C: 1% HCOOH in Water

Flow rate: 3.0 mL/min

Injection volume: 10 μ L

Sample concentration: 10 μ g/mL in water

Temperature: 30 °C

Detection: UV @ 254 nm


Instrument: Alliance 2695 with 2996 PDA


Gradient

Time	Profile		
(min)	%A	%B	%C
0.0	90	0	10
4.0	0	90	10

Results and Discussion

Compound mixture of phenones separated in under 4 minutes with SunFire IS Column.

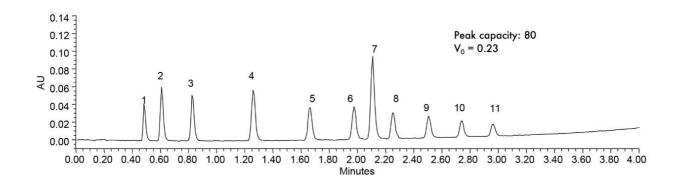

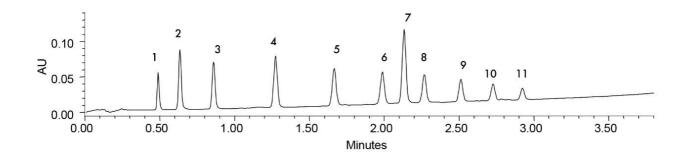

Featured Products

Alliance HPLC System https://www.waters.com/534293

WA41897, August 2005

© 2021 Waters Corporation. All Rights Reserved.