

Applikationsbericht

## Aflatoxins in Peanuts

---

YU Yanbin, WAN Shuwei, TAN Peigong, WANG Xiaogang, MIAO Zaijing

Ministry of Agriculture, Qingdao, Environmental Protection Agency, Qingdao, Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.

---

### Abstract

This application brief describes the analysis of aflatoxins in peanuts.

---

## Introduction

This application brief describes the analysis of aflatoxins in peanuts.

---


## Experimental

### Pretreatment

1. Add 5 g of sodium hydroxide to 20 g of homogenized sample, followed by 30 mL of n-hexane.
2. Add 100 mL 60% aqueous methanol and homogenize.
3. Ultrasonicate for 30 minutes.
4. Filter sample through 15 cm filter paper.
5. Take 1 mL aliquot from 60% methanol layer for SPE cleanup.

## SPE Procedure

Oasis® HLB 1cc/30 mg

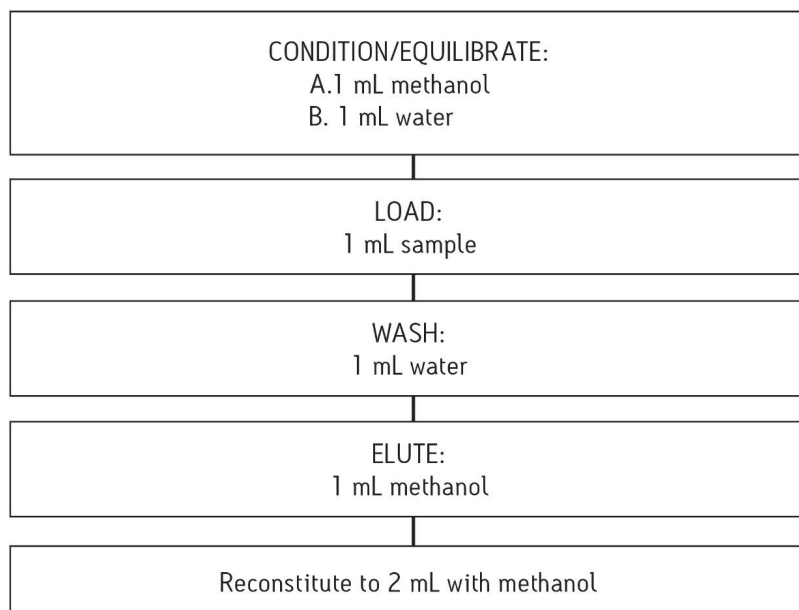


## LC Conditions

Instrument:	Alliance HPLC 2695 System
Column:	Symmetry Shield RP18, 4.6 x 150 mm, 5 µm
Flow rate of iodine:	0.2 mL
Flow rate:	1 mL/min
Mobile phase:	A. methanol B. water
Isocratic gradient:	35% A: 65% B, for 20 minutes
Column temperature:	30 °C
Derivatization temp.:	80 °C

Excitation wavelength:	365 nm
Emission wavelength:	455 nm
Post-column derivatization reagent:	Dissolve 200 mg iodine in 10 mL methanol, top up 1000 mL with water
Detector:	2475 Multi Wavelength Fluorescence

---

## Results and Discussion

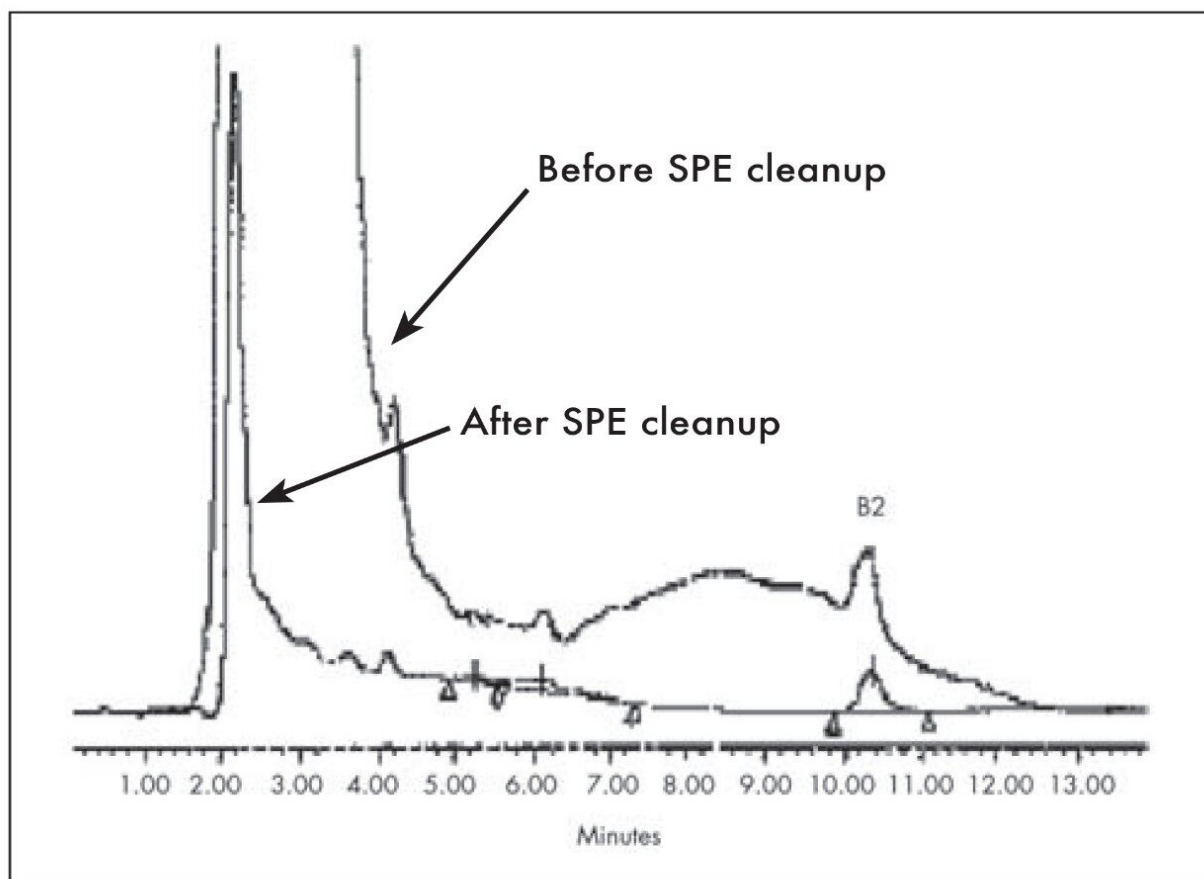

Matrix interference is greatly reduced when sample is cleaned up by using Oasis HLB SPE cartridge.

Analyte	Recovery %	Detection (p/μg kg)
Aflatoxin G2	101± 7.18	0.11
Aflatoxin G1	72.8±3.63	0.20
Aflatoxin B2	97.5±5.48	0.12
Aflatoxin B1	68.8±5.48	0.24

Results of B1, B2, G1, G2 in peanuts (n=5)

---

## Featured Products

Alliance HPLC System <<https://www.waters.com/534293>>

720002584, April 2008

© 2021 Waters Corporation. All Rights Reserved.