

Application Note

Analysis of Mono-, Di- and Oligosaccharides Using ACQUITY UPLC BEH Amide Columns

Waters Corporation



This is an Application Brief and does not contain a detailed Experimental section.

Abstract


This application brief describes the analysis of Oligosaccharides using ACQUITY UPLC BEH Amide Columns.

Introduction


Compounds used for this study includes:

1. p-Toluamide
2. Fructose
3. Glucose
4. Sucrose
5. Maltose
6. Maltotriose
7. Maltotetraose
8. Maltopentaose
9. Maltohexahose
10. Maltoheptaose


STRUCTURES

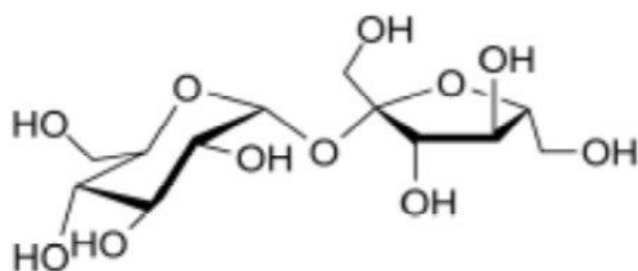


Sucrose

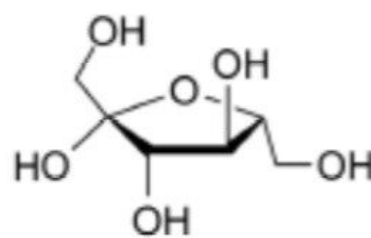


Fructose

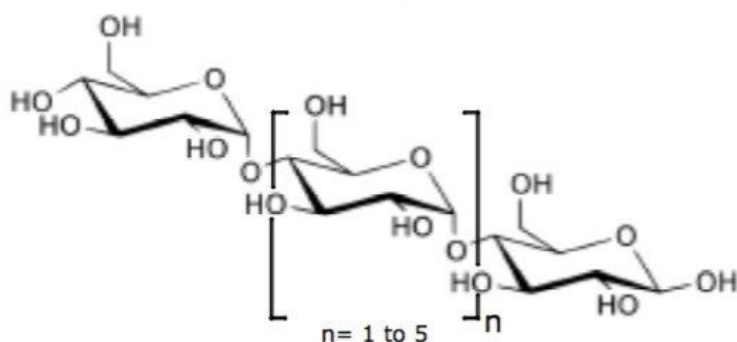


Maltooligosaccharides

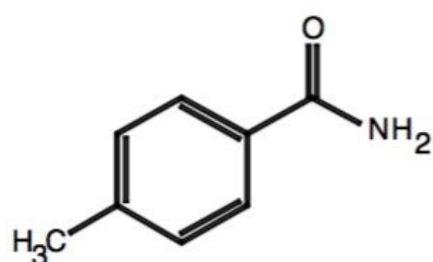

p-Toluamide
(unretained compound)

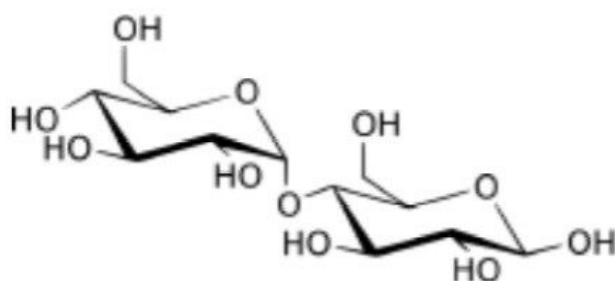

Maltose

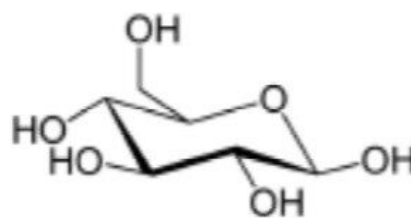

Glucose

Experimental

Chromatographic Conditions

Column:	ACQUITY UPLC BEH Amide 2.1 x 50 mm, 1.7 μ m	
Part Number:	186004800	
Mobile Phase A:	80/20 MeCN/H ₂ O with 0.05% triethylamine [TEA]	
Mobile Phase B:	30/70 MeCN/H ₂ O with 0.05% triethylamine [TEA]	
Flow Rate:	0.17 mL/min	
Gradient:	5 minute gradient, 80%-50% MeCN	
Injection Volume:	0.7 μ L (PLNO)	
Sample Concentration:	1 mg/mL each	
Sample Diluent:	50/50 MeCN/H ₂ O	
Column Temperature:	35 $^{\circ}$ C	
Strong Needle Wash:	20/80 MeCN/H ₂ O (800 μ L)	
Weak Needle Wash:	75/25 MeCN/H ₂ O (500 μ L)	
Seal Wash:	50/50 MeCN/H ₂ O	
Instrument:	Waters ACQUITY UPLC with ELSD	

Gradient:


Time (min)	%A	%B
0.00	100.00	0.00

Time (min)	%A	%B
5.00	40.00	60.00
5.01	100.00	0.00
15.00	100.00	0.00

ELSD Conditions

Gain:	200
Pressure:	40 psi
Drift Tube Temperature:	40 °C
Nebulizer:	Cooling
Data Rate:	10 pps
Filter Time Constant:	Normal

Results and Discussion

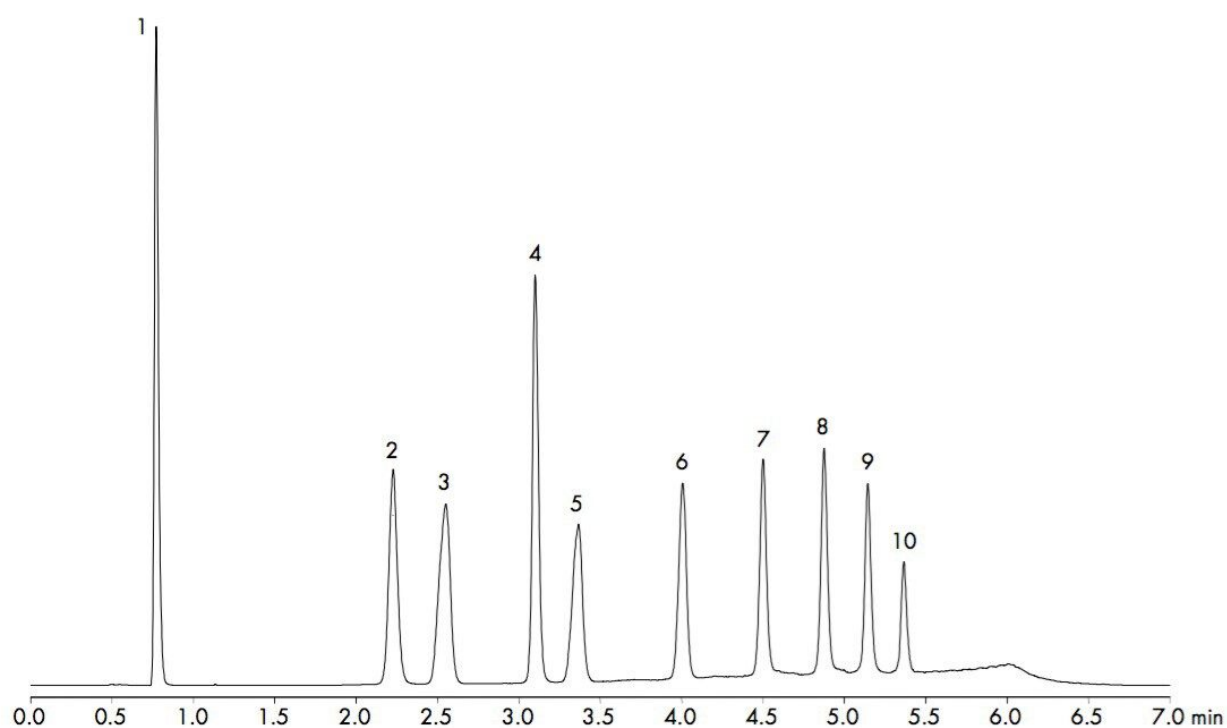

Featured Products

ACQUITY UPLC System <<https://www.waters.com/514207>>

ACQUITY UPLC ELS Detector <<https://www.waters.com/514219>>

WA60110, October 2009