

Analysis of Mono-, Di-, and Oligosaccharides Using ACQUITY UPLC BEH Amide Columns with Acetone as Organic Modifiers

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

Abstract

This application brief highlights the analysis of oligosaccharides using ACQUITY UPLC BEH Amide Columns with acetone as organic modifiers.


Introduction

Compounds used for this study includes:


1. p-Toluamide
 2. Fructose
 3. Glucose
 4. Sucrose
 5. Maltose
-

6. Maltotriose
7. Maltotetraose
8. Maltopentaose
9. Maltohexahose
10. Maltoheptaose


STRUCTURES

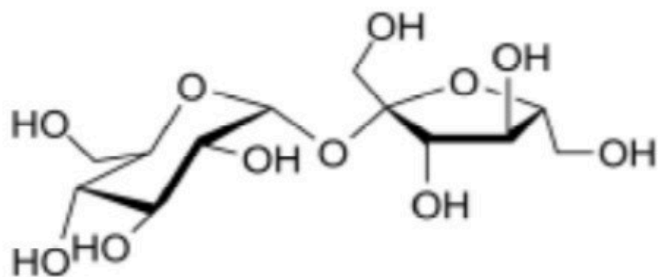


Sucrose

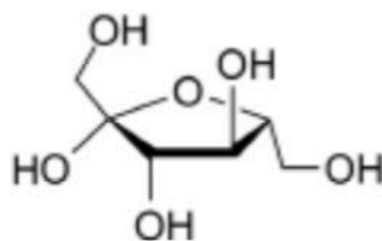


Fructose

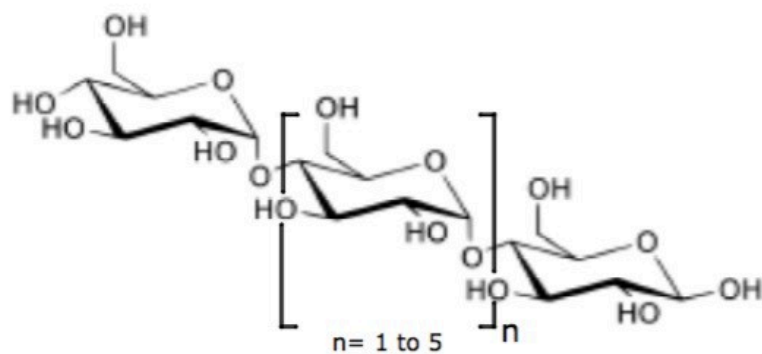


Maltooligosaccharides

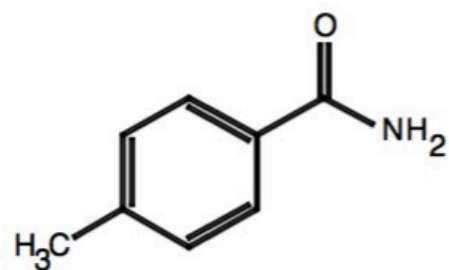

p-Toluamide
(unretained compound)

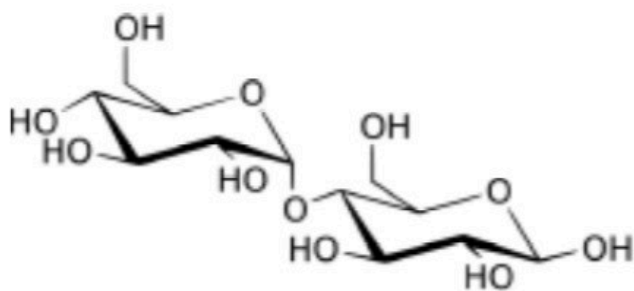

Maltose

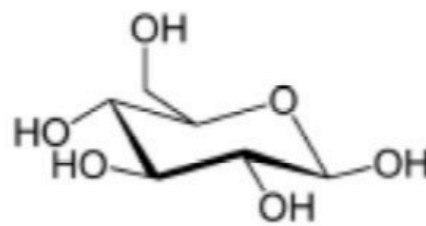

Glucose

Experimental

Chromatographic Conditions

Column:	ACQUITY UPLC BEH Amide 2.1 x 50 mm, 1.7 μ m
Part number:	186004800
Mobile phase A:	80/20 acetone/H ₂ O with 0.05% triethylamine [TEA]
Mobile phase B:	30/70 acetone/H ₂ O with 0.05% triethylamine [TEA]
Flow rate:	0.17 mL/min
Gradient:	5 minute gradient, 80%–60% MeCN with 10 minute re-equilibration
Injection volume:	0.7 μ L (PLNO)
Sample concentration:	1 mg/mL each
Sample diluent:	50/50 MeCN/H ₂ O
Column temperature:	85 $^{\circ}$ C
Strong needle wash:	20/80 MeCN/H ₂ O (800 μ L)
Weak needle wash:	75/25 MeCN/H ₂ O (500 μ L)
Seal wash:	50/50 MeCN/H ₂ O
Instrument:	Waters ACQUITY UPLC with ELSD


Gradient:

Time (min)	%A	%B
0.00	100.00	0.00
5.00	60.00	40.00
5.01	100.00	0.00
15.00	100.00	0.00

ELSD Conditions

Gain:	200
Pressure:	40 psi
Drift tube temperature:	40 °C
Nebulizer:	Cooling
Data rate:	10 pps
Filter time constant:	Normal

Results and Discussion

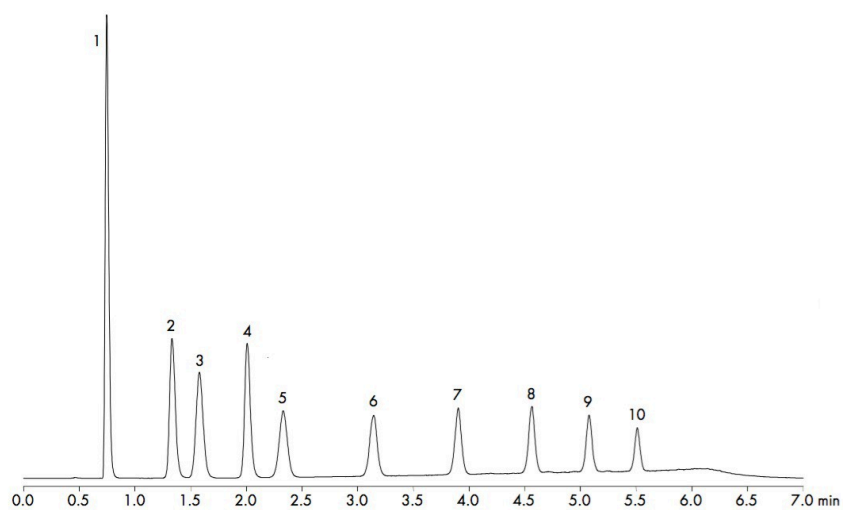

Featured Products

ACQUITY UPLC ELS Detector <<https://www.waters.com/514219>>

WA60111, October 2009

© 2022 Waters Corporation. All Rights Reserved.