

응용 자료

## Analysis of Mono-, Di-, and Oligosaccharides Using ACQUITY UPLC BEH Amide Columns with Acetone as Organic Modifiers

---

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

---

### Abstract

This application brief highlights the analysis of oligosaccharides using ACQUITY UPLC BEH Amide Columns with acetone as organic modifiers.

---


### Introduction

Compounds used for this study includes:


1. p-Toluamide
  2. Fructose
  3. Glucose
-

4. Sucrose
5. Maltose
6. Maltotriose
7. Maltotetraose
8. Maltopentaose
9. Maltohexahose
10. Maltoheptaose


## STRUCTURES

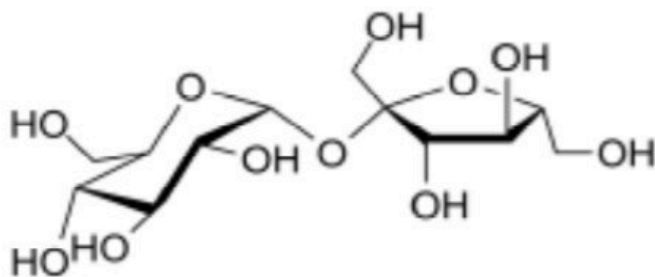


Sucrose

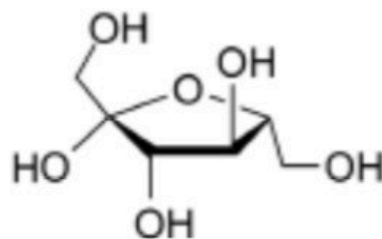


Fructose

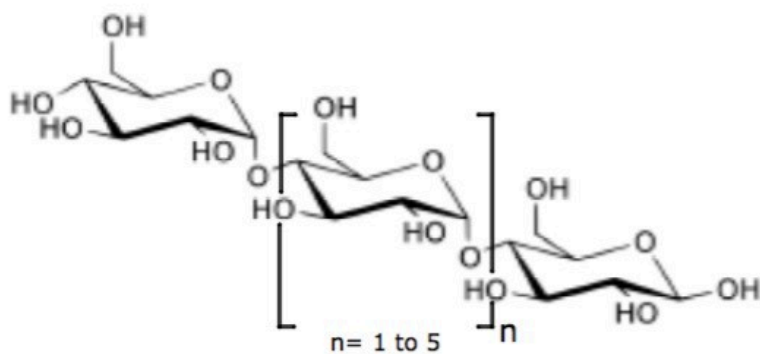


Maltooligosaccharides

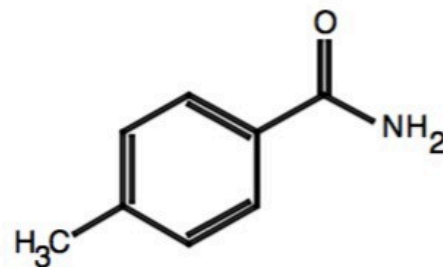

p-Toluamide  
(unretained compound)

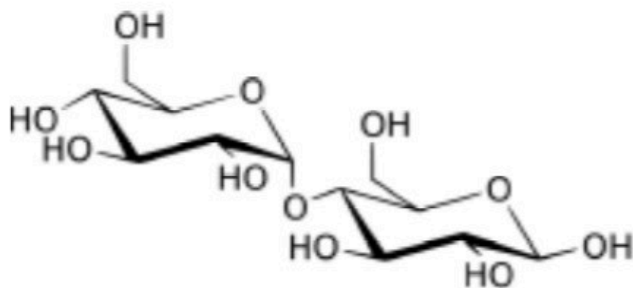

Maltose

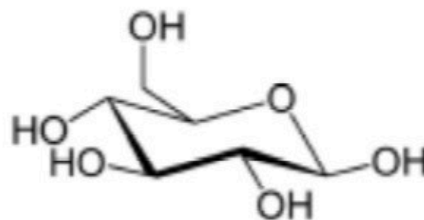

Glucose

---

## Experimental

### Chromatographic Conditions

Column:	ACQUITY UPLC BEH Amide 2.1 x 50 mm, 1.7 $\mu$ m
Part number:	186004800
Mobile phase A:	80/20 acetone/H <sub>2</sub> O with 0.05% triethylamine [TEA]
Mobile phase B:	30/70 acetone/H <sub>2</sub> O with 0.05% triethylamine [TEA]
Flow rate:	0.17 mL/min
Gradient:	5 minute gradient, 80%–60% MeCN with 10 minute re-equilibration
Injection volume:	0.7 $\mu$ L (PLNO)
Sample concentration:	1 mg/mL each
Sample diluent:	50/50 MeCN/H <sub>2</sub> O
Column temperature:	85 °C
Strong needle wash:	20/80 MeCN/H <sub>2</sub> O (800 $\mu$ L)
Weak needle wash:	75/25 MeCN/H <sub>2</sub> O (500 $\mu$ L)
Seal wash:	50/50 MeCN/H <sub>2</sub> O

Instrument:

Waters ACQUITY UPLC with ELSD

## Gradient:

Time (min)	%A	%B
0.00	100.00	0.00
5.00	60.00	40.00
5.01	100.00	0.00
15.00	100.00	0.00


## ELSD Conditions

Gain:	200
Pressure:	40 psi
Drift tube temperature:	40 °C
Nebulizer:	Cooling
Data rate:	10 pps
Filter time constant:	Normal

---

## Results and Discussion

---

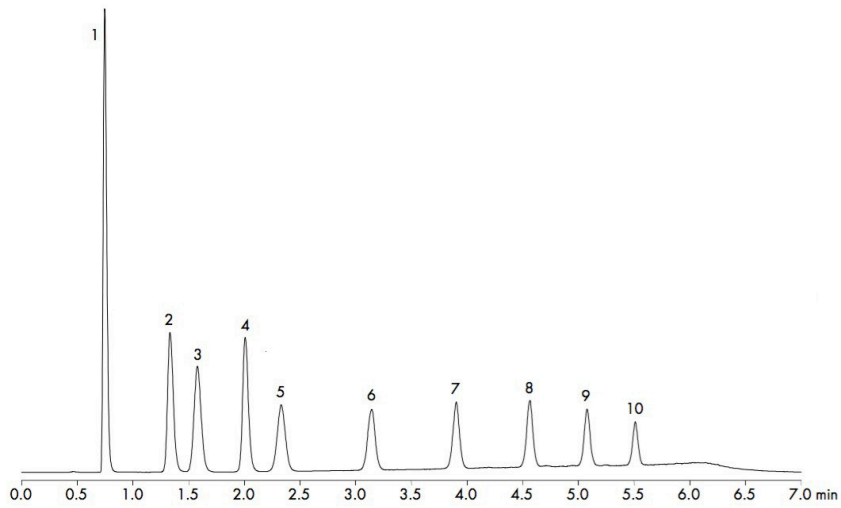

---

## Featured Products

ACQUITY UPLC ELS Detector <<https://www.waters.com/514219>>

WA60111, October 2009

© 2022 Waters Corporation. All Rights Reserved.