

An Inter-Laboratory Evaluation of a Confirmatory Method For Dioxins in Food and Environmental Samples Using APGC-MS/MS

Bert van Bavel, Dawei Geng, Laura Cherta, Jaime Nacher-Mestre, Tania Portolés, Abaos Abalos, Jordi Saulo, Esteban Abad, Jody Dunstan, Rhys Jones, Alexander Kotz, Helmut Winterhalter, Rainer Malisch, Wim Traag, Jessika Hagberg, Ingrid Ericson Jogsten, Joaquim Beltran, Felix Hernandez, Eimear McCall

MTM Research Centre, Örebro University, Research Institute for Pesticides and Water (IUPA), University Jaume I, Laboratory of Dioxins, IDAEA-CSIC, EU Reference Laboratory (EU-RL) for Dioxins and PCBs in Feed and Food, State Institute for Chemical and Veterinary Analysis of Food, Waters Corporation, RIKILT Institute of Food Safety, Wageningen University and Research Centre

Abstract

This application note demonstrates confirmatory GC-MS/MS method for the analysis of complex PCDDs and PCDFs in foods and feeds that is in compliance with recent EU Regulation 589/2014. The use of APGC in combination with the Xevo TQ-S for the analysis of dioxins has the same potential, in terms of sensitivity and selectivity, as the traditional HRMS instrumentation used for this analysis, and that it is compliant with Regulation 589/2014/EU.

Benefits

- Confirmatory analysis for dioxins at regulatory limits in food and feed.
- Proven regulatory compliance of APGC and Xevo TQ-S by multiple laboratories and analysts.

- Robust and accurate quantification of dioxins in food and environmental samples.
- Excellent agreement with existing GC-EI-HRMS results.

Introduction

The term dioxins refers to a group of chemically similar congeners, polychlorinated dibenzo-p-dioxins (PCDDs) and polychlorinated dibenzofurans (PCDFs), known to persist in the environment and pose significant toxicological concern. Therefore, they are well regulated and testing is enforced globally. Testing has been traditionally performed by GC-EI-HRMS. However, recent technological advances have allowed for a revision of the analytical criteria. Following extensive review, the European Commission has enacted Regulation 589/2014, which permits the use of GC-MS/MS for the confirmatory analysis of dioxins in food and feed.¹

In this application note, we summarize a comprehensive study completed by van Bavel, et al. that demonstrates the capabilities of Waters Atmospheric Pressure Gas Chromatography (APGC), coupled with Xevo TQ-S for the determination of dioxins in a variety of sample matrices. The performance of APGC was compared to samples previously characterized by GC-HRMS, the gold standard in dioxin analysis. Finally, system robustness was investigated by an inter-laboratory comparison trial using four different Xevo TQ-S systems with APGC. A more detailed description of the method and results achieved are described by van Bavel *et al.*²

Experimental

GC conditions

GC system:	7890A
Column:	DB-5MS (60 m x 0.25 mm id. x film thickness 0.25 μm) or BPX-5 (30 m x 0.25 mm I.D. x 0.25 μm)

Injection:	1 μL pulsed splitless mode (at 280°C) or 5 μL MMI PTV (at 100 °C, 0.5 min; 340 °C, 20 min)
Transfer line temp.:	280 °C to 360 °C
Carrier gas flow:	1.4 to 2 mL. min ⁻¹ (helium)
Auxiliary gas:	250 to 300 L. h ⁻¹ (nitrogen)
Make-up gas:	150 to 370 mL. min ⁻¹ (nitrogen)

MS conditions

MS system:	Xevo TQ-S
Corona pin:	1.8 to 2.1 μA
Source temp.:	150 °C
Cone gas flow:	170 to 200 L.h ⁻¹
Collision gas:	2.5 to 6.2 x 10 ⁻³ mbar (argon)
Acquisition:	MRM mode, as shown in Table 1
Quantitative analysis was performed in MRM mode	
Data management:	MassLynx MS Software, v4.1, with TargetLynx Application Manager

Standards

EPA-1613 CSL to CS5 Standards, containing both native and ¹³C labelled PCDD, PCDF and TCDD compounds, were used for calibration curves. For method performance and sample preparation the following

standards were used: EPA-1613 PAR, EPA-1613 LCS and TF-TCDD-MXB, along with ¹³C- labelled EPA-1613 ISS PCDD and PCDF congeners. All standards were purchased from Wellington Laboratories (Ontario, Canada). A further dilution of the CSL standard was made in nonane to give a 10 fg.µl⁻¹ standard.

Sample preparation

A wide variety of characterized samples were investigated in this study. Certified reference materials of BCR-607 (milk powder), BCR-677 (sewage sludge), and BCR 490 and BCR-615 (fly ash) were acquired from the Institute for Reference Materials and Measurements (IRMM), European Commission Joint Research Centre (Geel, Belgium). Internal reference materials for routine quality control in the four laboratories: human blood and naturally contaminated food and feed samples, international intercomparison studies (fish), and proficiency tests organized by the EU reference laboratory were also used to compare results from different systems. Samples were prepared following previously validated methods, standard methods, or based on analytical criteria of the EU Commission.³⁻⁷

Instrument conditions

A summary of the instrument conditions used across the four different laboratories are provided here. More specific APGC-TQ-S instrument conditions are detailed by Dunstan *et al.*⁸

Results and Discussion

The analysis of dioxins and furans was completed using the Xevo TQ-S with APGC across four different laboratories: 1. Örebro University, Örebro, Sweden; 2. University Jaume I, Castellón and IAEA-CSIC, Barcelona, Spain; 3. EURL for Dioxins and PCCBs in Feed and Food, Freiburg, Germany, and 4. Waters, Manchester, UK. Following instrument optimization, an inter-laboratory comparison was performed using certified reference materials. These results were further compared to those obtained by the traditional GC-HRMS technique.

MRM selectivity and specificity

APGC-MS/MS ionization under charge-transfer conditions (dry source) revealed an abundant presence of the molecular ion for all 17 of the 2,3,7,8 chlorine substituted dioxins and furans. Therefore, MS/MS scans were performed in order to find selective transitions based on the use of M+• as precursor ion.

Collision energies of 30 and 40 eV were selected for all of the PCDDs and PCDFs, respectively, and are summarized in Table 1. At low collision energies, the product ion spectrum was dominated by the ^{35}Cl loss, but at the final optimum collision energies, the transitions selected corresponded to the loss of $[\text{CO}^{35}\text{Cl}]$. This fragmentation is very specific for dioxins and furans, providing beneficial selectivity.

Compound	Precursor ion (m/z)	Product ion (m/z)	Collision energy (eV)
TCDF	304	241	40
	306	243	40
¹³ C TCDF	316	252	40
	318	254	40
TCDD	320	257	30
	322	359	30
¹³ C TCDD	332	268	30
	334	270	30
PCDF	338	275	40
	340	277	40
¹³ C PCDF	350	286	40
	352	288	40
PCDD	354	291	30
	356	293	30
¹³ C PCDD	366	302	30
	368	304	30
HxCDF	374	311	40
	376	313	40
¹³ C HxCDF	386	322	40
	388	324	40
HxCDD	390	327	30
	392	329	30
¹³ C HxCDD	402	338	30
	404	340	30
HpCDF	408	345	40
	410	347	40
¹³ C HpCDF	420	356	40
	422	358	40
HpCDD	424	361	30
	426	363	30
¹³ C HpCDD	436	372	30
	438	374	30
OCDF	442	379	40
	444	381	40
OCDD	458	395	30
	460	397	30
¹³ C OCDD	470	406	30
	472	408	30

Table 1. MRM transitions for MS/MS mode.

Analytical performance

Analytical performance was evaluated across four different laboratories investigating detection limit, linearity, ion ratios, repeatability, and reproducibility of the method. For ease of interpretation, these parameters are compared to HRMS requirements presented in EPA1613 or EN 16215 for dioxin analysis.

The sensitivity for all tetra- to octa-substituted PCDD/DFs was investigated. TeCDD/TeCDF, PeCDD/PeCDF/HxCDF/ HxCDD/HpCDD/HpCDF, and OCDD/OCDF were analyzed at 10, 50, and 100 $\text{fg}\cdot\mu\text{l}^{-1}$ respectively, as shown in Figure 1.

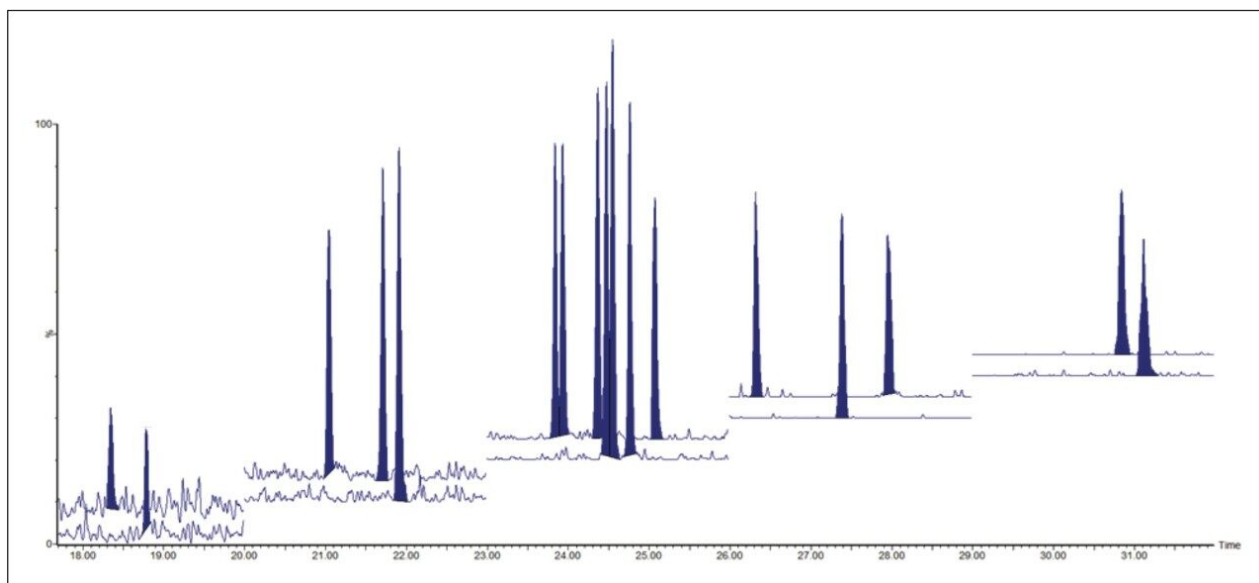


Figure 1. Example of chromatographic separation achieved for 17 PCDD/DF congeners at 1 in 10 dilution of the CSL standard.

Typically for the evaluation of high resolution mass spectrometry instruments a 100 $\text{fg}\cdot\mu\text{l}^{-1}$ standard of 2,3,7,8-TeCDD is monitored, where a signal-to noise (S/N) ratio of >100 is required. Therefore, following the initial setup of the APGC-Xevo TQ-S, the lowest calibration point for 2,3,7,8-TeCDD in this method was diluted to 10 $\text{fg}\cdot\mu\text{l}^{-1}$. This solution readily achieved a S/N ratio of >50 in all four laboratories, well below the required limit.

The ultimate sensitivity was tested using a mixture of TCDD congeners (TF-TCDD-MXB) at concentrations of 2, 5, 10, 25, 50, and 100 $\text{fg}\cdot\mu\text{l}^{-1}$ where 2 $\text{fg}\cdot\mu\text{l}^{-1}$ on column allowed for satisfactory detection of the congeners, as shown in Figure 2. All of these results are impressive and in good agreement with, or even better than those routinely achieved with high resolution magnetic sector GC-MS systems.

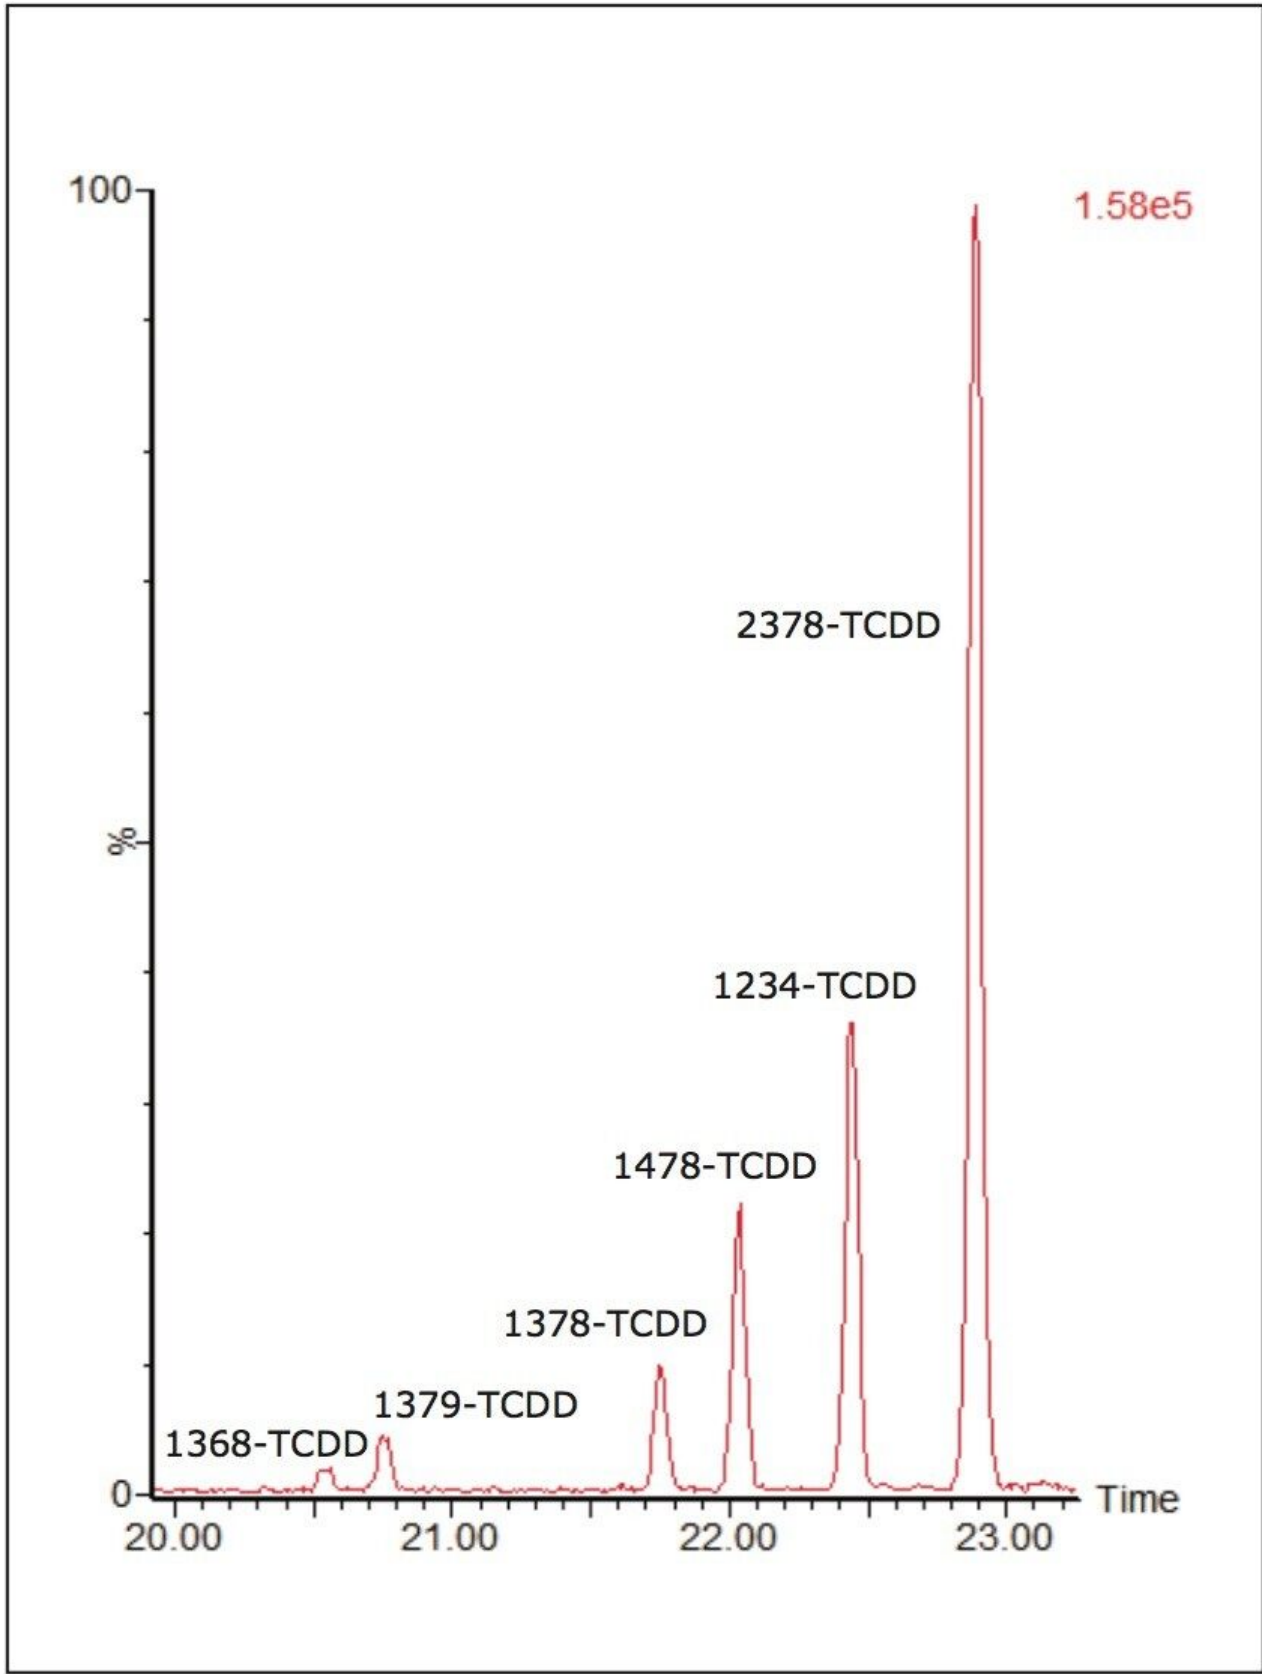


Figure 2. Chromatographic separation of TCDD congener mix containing 2 to 100 pg (concentration on column, with 1 μ l injected).

The linearity of the method was studied by analyzing the standard solutions (in triplicate) at six concentrations, ranging from 0.1 to 40 $\text{pg}\cdot\mu\text{l}^{-1}$ (EPA-1613 CSL to CS4) on the four different systems. The linearity, using internal standard calibration, was satisfactory with coefficient of determination (R^2) >0.998. The relative standard deviation (RSD) of the relative response factors (RRFs), as defined in standard methods EPA 1613 or EU 1948, was also achieved (*i.e.* below 15%), as required by both methods. Based on area, the repeatability was within 15% for the injection of 10 $\text{fg}\cdot\mu\text{l}^{-1}$ (n=3-10), and below 10% for all PCDD/DFs for the CSL standard against the corresponding ^{13}C standard (RRF).

An important criterion for the unequivocal identification of the PCDD/F congeners is the ion abundance ratio between the two monitored product ions, resulting from two different precursor ions. For quality control, the ion abundance ratios can be compared with calculated or measured values. The calculated ratio depends on the relative abundance of the two selected precursor ions ($[\text{M}+\cdot\ ^{35}\text{Cl}]$ and $[\text{M}+\cdot\ ^{37}\text{Cl}]$), and their relative loss of $[\text{CO}^{35}\text{Cl}]$ or $[\text{CO}^{37}\text{Cl}]$ that result in the formation of each product ion. It is only comparable with the measured ratios, if identical collision energy and collision gas pressure is applied for both transitions. The measured ion abundance ratios in the sample extracts matched those of the calibration standards within the QC limits of $\pm 15\%$, as derived from EPA 1613 for HRMS and EU Regulation 589/2014.

The ion abundance ratios, in combination with the relative response factors from the calibration curves can further be used to check the reliability of the results in the low concentration range. Limits of quantification (LOQs) were determined based on maximum deviations ($\pm 15\%$) of the calculated value for ion abundance ratios and deviations ($\leq 30\%$) of the relative response factor of the mean value. With an RSD of $\leq 20\%$ for the complete calibration, LOQs in the range of 10 to 30 fg (on column) were obtained for 2,3,7,8-TCDD and 2,3,7,8-TCDF.

Comparison of APGC-MS/MS and GC-HRMS results

In order to test the capabilities of the developed method, proficiency samples outlined in the experimental section were previously run and characterized on high resolution systems. These samples were re-injected on the APGC-MS/MS system in three different laboratories: the EURL for Dioxins and PCBs in Germany, CSIC and IUPA in Spain, and MTM in Sweden. Each laboratory tested different samples by GC-HRMS and APGC-MS/MS, as shown in Figure 3. Excellent correlation between the instruments was demonstrated, where the relative difference between the APGC and the HRMS results <7% for all samples. Like HRMS, the

APGC runs passed all QA/QC criteria in terms of chromatographic separation, linearity, S/N ratio, and ion abundance ratio of selected transitions.

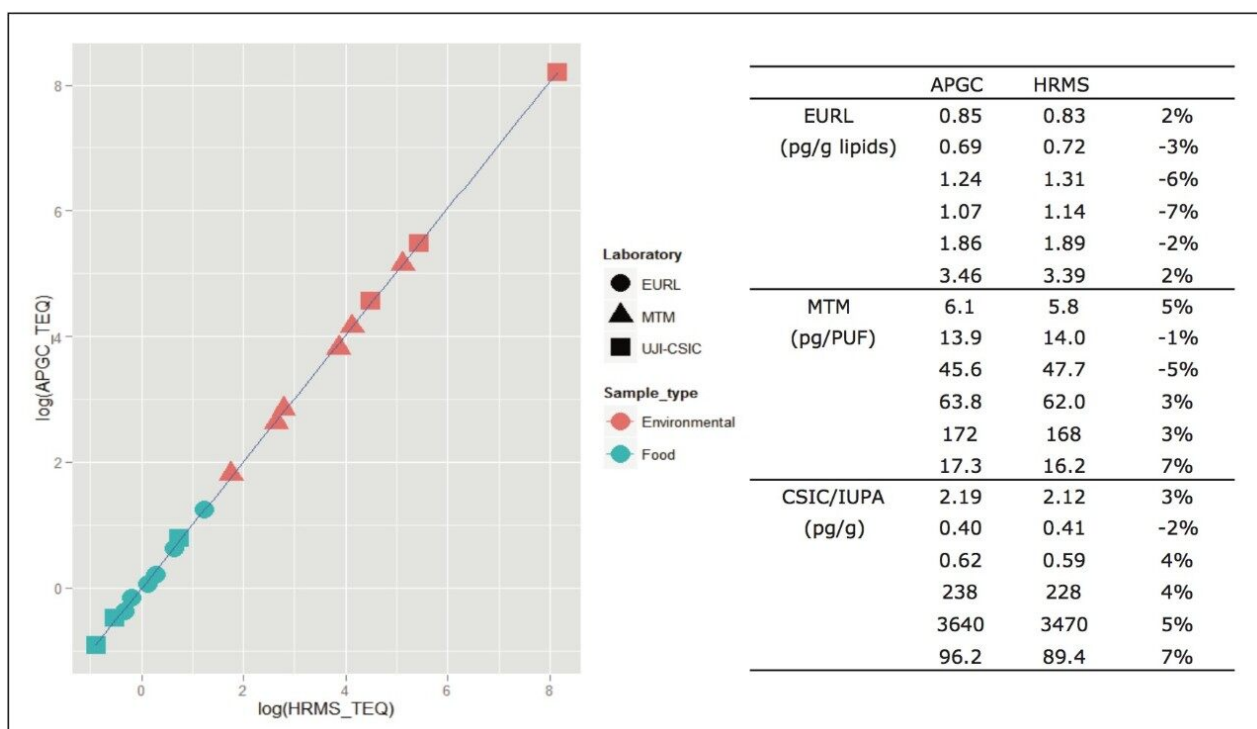


Figure 3. Comparison of APGC-MS/MS results and GC-EI-HRMS for different samples analyzed by three different laboratories. Good agreement was observed for dioxins in food and environmental samples, where a variance of $\leq 7\%$ was determined between techniques for all samples.

An additional summary of quality control food samples analysed by both GC-HRMS and APGC-TQ-S is given in Figure 4. Excellent correlation is evident between the two techniques, over a wide concentration range and in a variety of food matrices.

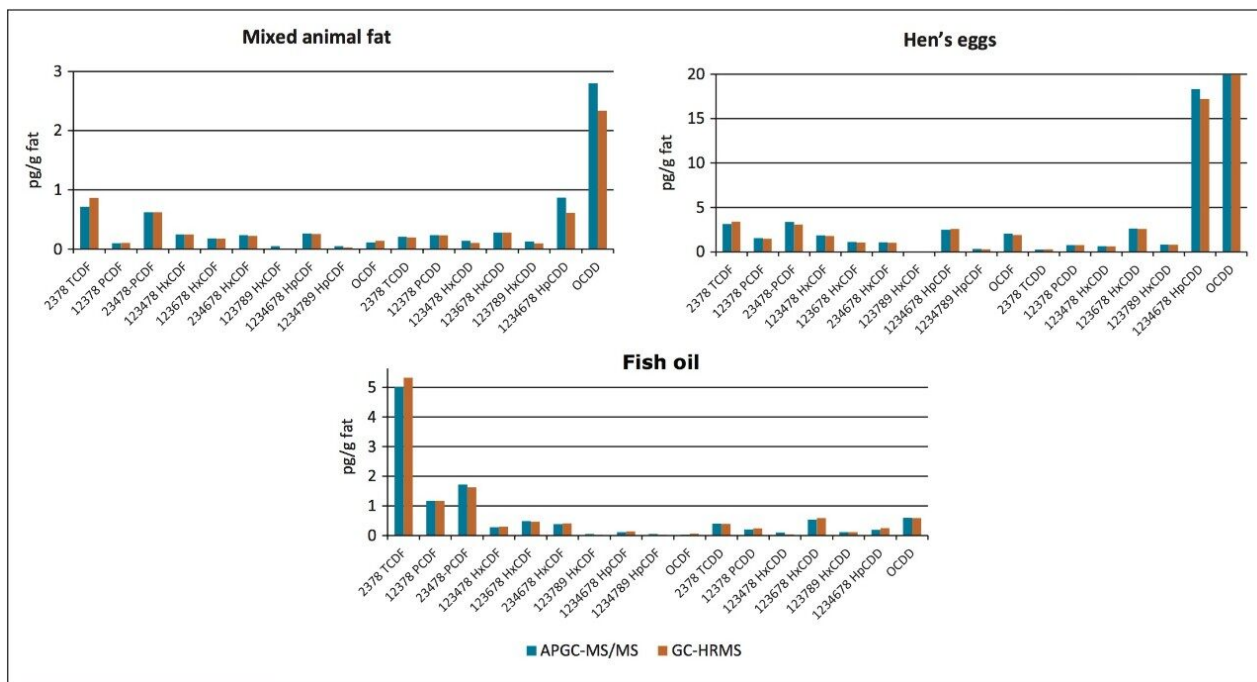


Figure 4. Comparison of results obtained from APGC-MS/MS and GC-HRMS for a sample matrix of mixed animal fat, fish oil, and hen's eggs.

Conclusion

The potential of using APGC-TQ-S for the identification and quantification of dioxins and furans in a variety of complex matrices has been successfully demonstrated. Following the recent change to analytical criteria in EU Regulation 589/2014, GC-MS/MS can now be used as a confirmatory method for the analysis of PCDDs and PCDFs in foods and feeds.

Van Bavel, *et al.* have demonstrated that the results of the APGC system are impressive and comparable with HRMS not only in selectivity but also in sensitivity.² Excellent linearity was achieved ($R^2 > 0.998$) over an appropriate calibration range.

The results from a wide variety of complex samples previously analyzed by GC-(EI)-HRMS were compared with the results from the APGC-MS/MS system. Results between instruments showed excellent agreement, both in terms of the individual congeners and toxic equivalence factors (TEQs).

The authors conclude that the use of APGC in combination with the Xevo TQ-S for the analysis of dioxins has

the same potential, in terms of sensitivity and selectivity, as the traditional HRMS instrumentation used for this analysis, and that it is compliant with Regulation 589/2014/EU. The APGC-MS/MS benchtop system, however, is far easier to use, maintain, and it can be quickly converted for liquid chromatography analysis.

References

1. European Commission, European Union Regulation No. 589, 2014, *Off. J. Eur. Union*.
2. van Bavel B, Geng D, Cherta L, Nácher-Mestre J, Portolés T, Ábalos M, Sauló J, Abad E, Dunstan J, Jones R, Kotz A, Winterhalter H, Malisch R, Traag W, Hagberg J, Ericson Jogsten I, Beltran J, Hernández F. 2015, *Anal Chem*. 10.1021/acs.analchem.5b02264, 2015.
3. Abad E, Saulo J, Caixach J, Rivera J., 2000, *J Chrom A*. 893 (2), 383–391.
4. U.S. Environmental Protection Agency. www.epa.gov, 1–89, 1994.
5. EN 16215:2012 European Standard EN 16215, European committee for standardisation, www.cen.eu, 2012.
6. European Commission, Commission Regulations (EU) No. 252, 2012, *Off. J. Eur. Union*.
7. European Commission, Commission Regulations (EU) No. 152, 2009, *Off. J. Eur. Union*.
8. Dunstan J, McCall E, Rao R, Ericson Jorgsten I, van Bavel B. A Confirmatory Method for PCDDs and PCDFs in Compliance with EU Regulation 589/2014/EU Using Atmospheric Pressure Gas Chromatography (APGC) with Xevo TQ-S. Waters application note no. 720005431en, June 2015.

Featured Products

[Waters Atmospheric Pressure Gas Chromatography \(APGC\) <https://www.waters.com/10100362>](https://www.waters.com/10100362)

[Xevo TQ-S <https://www.waters.com/10160596>](https://www.waters.com/10160596)

[MassLynx MS Software <https://www.waters.com/513662>](https://www.waters.com/513662)

[TargetLynx <https://www.waters.com/513791>](https://www.waters.com/513791)

720005219, November 2015

©2019 Waters Corporation. All Rights Reserved.