

Application Note

Determination of Triphenylmethane Dyes and their Metabolites in Shrimp Using QuEChERS Extraction and the ACQUITY UPLC H-Class System with Xevo TQD

Elizabeth Brady, Jennifer A. Burgess

Waters Corporation



Abstract

The practice of farming aquatic species has seen significant growth as certain areas of the world's fish stock become overexploited. One of the main challenges in the aquaculture industry is the control of infectious diseases.

Due to their efficacy and low cost, triphenylmethane (TPM) dyes including malachite green (MG), crystal violet (CV), and brilliant green (BG) have been implemented to combat this problem. Originally used as textile and paper dyes, they were introduced to aquaculture in 1933 as antibacterial, antifungal, and antiparasitic agents.

Both MG and CV are easily absorbed and known to metabolize to the equivalent, colorless leuco-forms, leucomalachite green (LMG) and leucocrystal violet (LCV), which are also mutagenic.

These compounds accumulate in fish and when this contaminated seafood is consumed by humans it poses a potential health risk. In addition to the toxic effects demonstrated in animal studies, these dyes have not been registered as veterinary drugs and have been banned for use in aquaculture by many countries.

In this application note, we report a highly sensitive and efficient LC-MS/MS method for simultaneously analyzing triphenylmethane (TPM) dyes in shrimp.

Benefits

- Simultaneous analysis of triphenylmethane dyes in aquaculture products using the ACQUITY UPLC H-Class System and Xevo TQD
- A modified QuEChERS sample preparation procedure provides a fast and efficient method for accurately analyzing seafood matrices resulting in little to no matrix effects.

Introduction

Motivated by the various potential health benefits, global consumption of seafood continues to increase. In order to meet this demand, the practice of farming aquatic species has seen significant growth as certain areas of the world's fish stock become overexploited. One of the main challenges in the aquaculture industry is the control of infectious diseases. Due to their efficacy and low cost, triphenylmethane (TPM) dyes

including malachite green (MG), crystal violet (CV), and brilliant green (BG) have been implemented to combat this problem. Originally used as textile and paper dyes, they were introduced to aquaculture in 1933 as antibacterial, antifungal, and antiparasitic agents.¹ Both MG and CV are easily absorbed and known to metabolize to the equivalent, colorless leuco-forms, leucomalachite green (LMG) and leucocrystal violet (LCV), which are also mutagenic.

These compounds accumulate in fish and when this contaminated seafood is consumed by humans it poses a potential health risk. In addition to the toxic effects demonstrated in animal studies, these dyes have not been registered as veterinary drugs and have been banned for use in aquaculture by many countries. Despite these bans, the frequent occurrence of TPM dye residue in seafood products has resulted in emergency measures to test imports, import bans, and product recalls. In the United States MG and CV are monitored to a detection limit of 1 µg/kg, whereas the EU has implemented a minimum required performance limit (MRPL) for the sum of MG and LMG of 2 µg/kg.^{2,3} Sensitive and selective methods are needed to monitor the presence of TPM dyes in aquaculture products as an important means of monitoring the safety of seafood and managing global health risks.

Preparation for the simultaneous analysis of TPM dyes in aquaculture samples typically includes aqueous or organic solvent extractions and several cleanup steps including solid phase extractions. These methods, however, can be tedious, time consuming and costly. To address these concerns, a modified QuEChERS technique was employed for preparation of shrimp.⁴

Experimental

UPLC conditions

UPLC system:	ACQUITY UPLC H-Class
Mobile phase A:	Water + 20 mmol ammonium acetate adjusted to pH 4 with acetic acid
Mobile phase B:	Acetonitrile
Column:	ACQUITY UPLC BEH C ₁₈ 2.1 x 100 mm, 1.7 µm

Column temp.: 40 °C
Injection volume: 5 µL
Flow rate: 0.3 mL/min
Total run time: 6 min

Gradient

Time	%A	%B
Initial	70	30
0.25	50	50
0.67	5	95
2.67	5	95
2.68	70	30
6.00	70	30

MS conditions

MS system: Xevo TQD
Ionization mode: ES+
Capillary voltage: 2.5 kV
Source temp.: 150 °C
Desolvation temp.: 400 °C

Desolvation gas: 780 L/hr

Acquisition: Multiple Reaction Monitoring (MRM)

The most commonly employed form of analysis for TPM dyes in seafood is high performance liquid chromatography (HPLC) coupled to an optical detector or mass spectrometer. The use of mass spectrometry avoids the need for a post column oxidation step which is necessary with UV/Vis detection to convert leuco forms to their parent compounds for simultaneous analysis. LC-MS/MS is now more commonly used for the detection, identification, and quantification of TPM dyes and residues as it meets the EU Commission Decision 657/2002/EC.

In this application note, we report a highly sensitive and efficient LC-MS/MS method for simultaneously analyzing MG, LMG, CV, LCV, and BG using the Waters ACQUITY UPLC H-Class System with the Xevo TQD.

Sample description

Shelled, headless tiger shrimp were homogenized in a blender and 10 g of homogenized shrimp were weighed out. 10 mL of acetonitrile with 1% acetic acid were added and the sample was shaken for 1 minute. A Waters DisQuE QuEChERS Pouch (p/n 186006812) containing 1.5 g sodium acetate and 6 g magnesium sulfate was added and shaken for 30 seconds. The mixture was placed in an ultrasonic bath for 12 minutes and centrifuged at 4000 rpm for 10 minutes at 15 °C. The supernatant was transferred to a 15-mL DisQuE QuEChERS PSA Tube (p/n 186004833) containing 900 mg magnesium sulfate, 150 mg primary secondary amine, and C₁₈. The sample was shaken for 1 minute and centrifuged at 4000 rpm for 5 minutes at 15 °C.

For pre spiked samples: 10 g of homogenized shrimp were spiked with 1 µg/kg of internal standards and 1 ppb of TPM dye mixture. After spiking, the sample was allowed to sit for 10 minutes to let the tissue and dyes interact. The sample preparation procedure described above was then carried out.

For post spiked samples: After the above procedure was performed on the unspiked shrimp samples, the resulting solution was spiked with the appropriate concentration of TPM dyes and 1 µg/kg of internal standards. Matrix matched calibration standards ranged from 0.05 to 40 ppb.

Solvent calibration standards were created by making dilutions in acetonitrile from 0.05 to 40 ppb.

Acquisition and processing methods

For each analyte, two MRM transitions were acquired. The most intense transition was used for quantification and the second transition was used for identification. Two deuterated internal standards,

Leuomalachite Green D₅ (LMG-D₅) and Leucocrystal Violet D₆ (LCV-D₆) were incorporated into the analysis to evaluate their application as internal standards. The retention times, MRM transitions, cone voltages and collision energies of all analytes are given in Table 1. Chemical structures of all analytes are displayed in Figure 1. TargetLynx Software was used for all processing.

Compound	RT (min)	Precursor (m/z)	Cone voltage (V)	Product 1 (m/z)	Collision energy 1 (V)	Product 2 (m/z)	Collision energy 2 (V)
Malachite Green	2.30	329.2	70	313.8	35	208.6	50
Leuomalachite Green	3.28	331.3	50	239.3	30	316.4	20
Crystal Violet	2.48	372.4	75	356.5	40	251.3	35
Leucocrystal Violet	3.33	374.3	50	358.5	30	238.3	25
Brilliant Green	2.65	385.5	80	341.5	40	297.3	55
Leuomalachite Green D ₅	3.27	336.3	50	239.4	40	321.3	45
Leucocrystal Violet D ₆	3.31	380.2	50	364.7	30	361.3	35

Table 1. List of triphenylmethane dyes, retention times, MRM transitions, cone voltages, and collision energies.

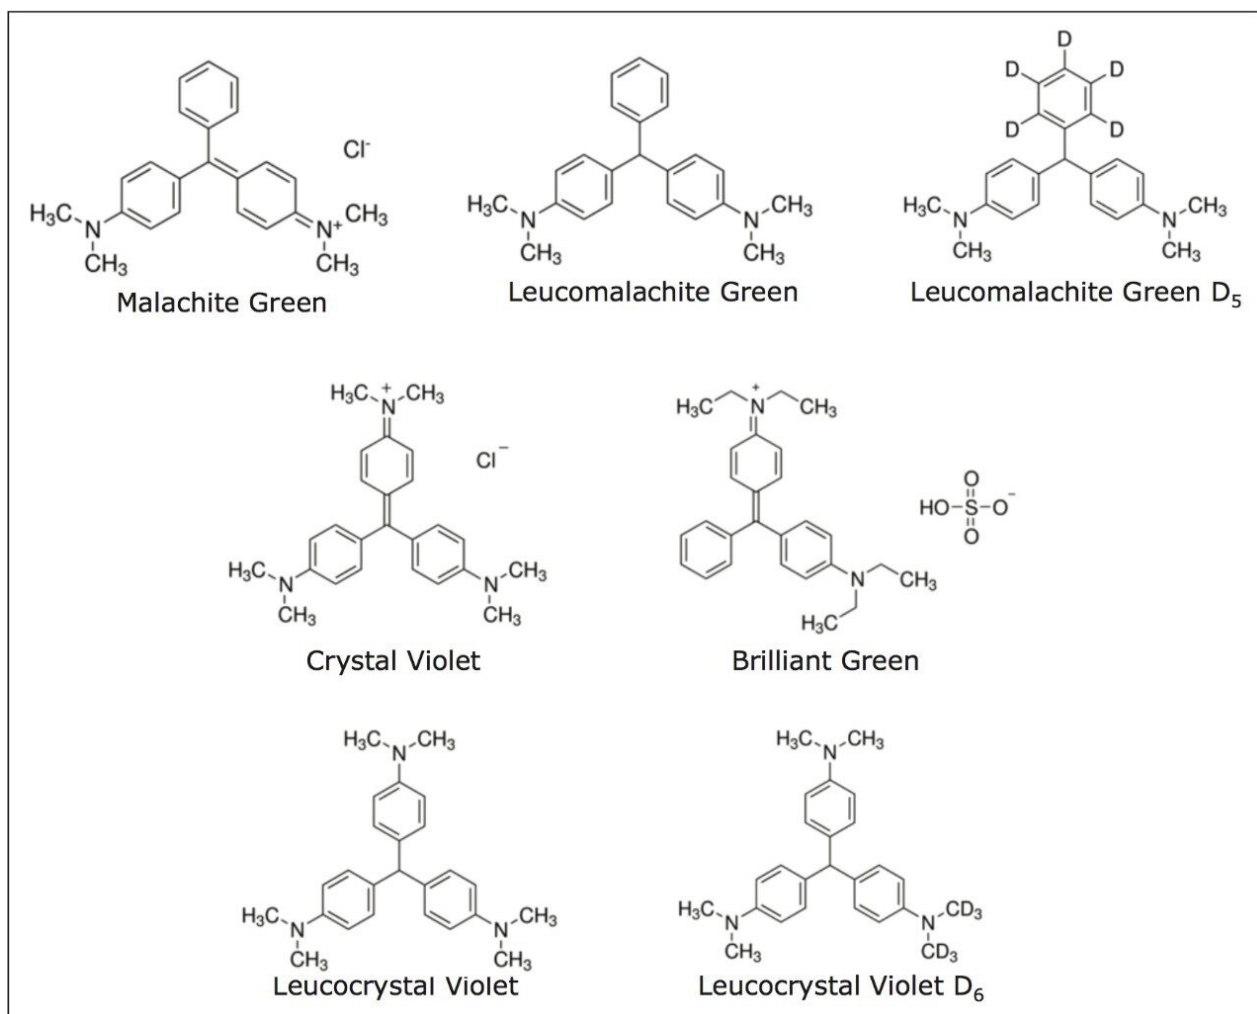


Figure 1. Chemical structures of the analytes.

Results and Discussion

Linearity and matrix effects

The chromatograms of each analyte at $1 \mu\text{g}/\text{kg}$ in a shrimp matrix shown in Figure 2 display the sensitivity obtained at the detection level monitored in the US. Excellent linearity was achieved for all compounds with all R^2 values greater than 0.998 as shown in Figure 3. The limits of the curves are ten to twenty times lower than the FDA limit of $1 \mu\text{g}/\text{kg}$. This was achieved without a concentration step in the sample preparation step demonstrating the sensitivity of this method. The matrix effects were calculated by comparing the slope of

the solvent calibration curves to those of the matrix matched calibration curves. The results are shown in Table 2.

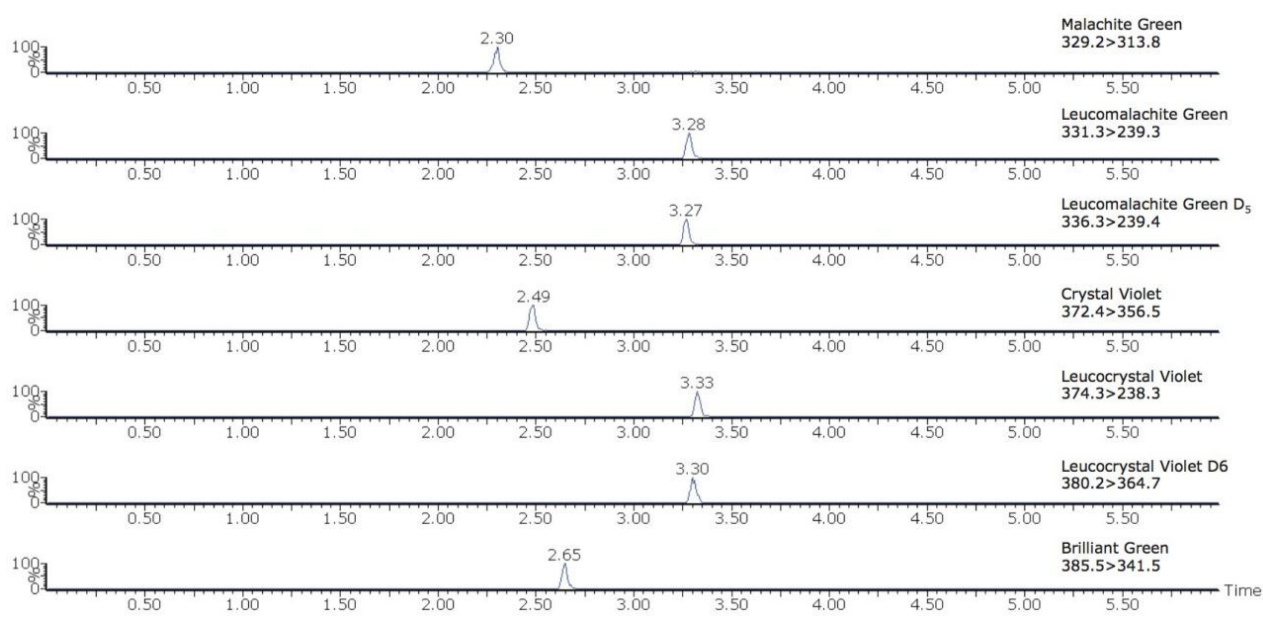


Figure 2. Chromatograms showing the primary MRM transitions for the three TPM dyes, two metabolites, and two internal standards at 1 µg/kg in shrimp matrix.


TPM dye	Slope ratio for shrimp matrix
Malachite Green	0.97
Leucomalachite Green	0.98
Crystal Violet	1.04
Leucocrystal Violet	1.19
Brilliant Green	0.95

Table 2. Matrix effects in shrimp.


A slope ratio value of 1 indicates no matrix effect, a value >1 indicates signal enhancement, and a value <1

indicates an effect of ion suppression. Most of the dyes showed little to no matrix effect while LCV showed a slight signal enhancement. This demonstrates the effectiveness of the QuEChERS sample preparation for the analysis of TPM dyes in seafood.


Compound name: Malachite Green
Correlation coefficient: $r = 0.999753$, $r^2 = 0.999506$
Calibration curve: $1315.24 * x + -17.4749$
Response type: External Std, Area
Curve type: Linear, Origin: Exclude, Weighting: 1/x, Axis trans: None

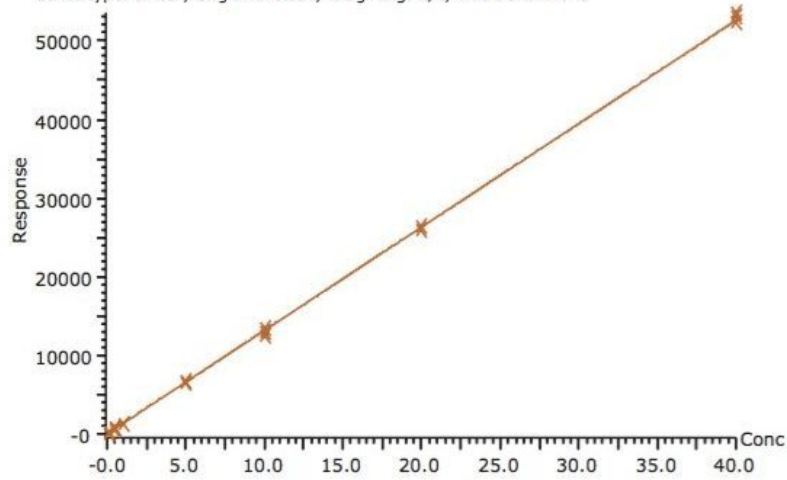

Compound name: Crystal Violet
Correlation coefficient: $r = 0.999889$, $r^2 = 0.999778$
Calibration curve: $2916.49 * x + 10.8663$
Response type: External Std, Area
Curve type: Linear, Origin: Exclude, Weighting: 1/x, Axis trans: None

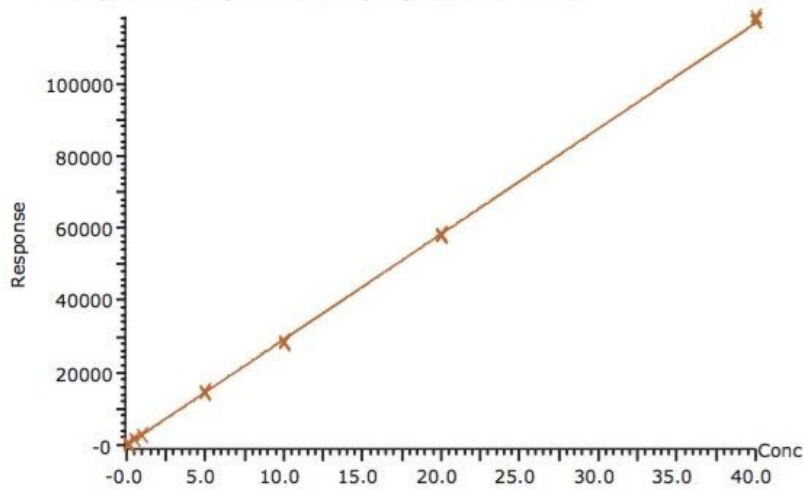

Compound name: Brilliant Green
Correlation coefficient: $r = 0.999886$, $r^2 = 0.999773$
Calibration curve: $1518.98 * x + -4.33236$
Response type: External Std, Area
Curve type: Linear, Origin: Exclude, Weighting: 1/x, Axis trans: None

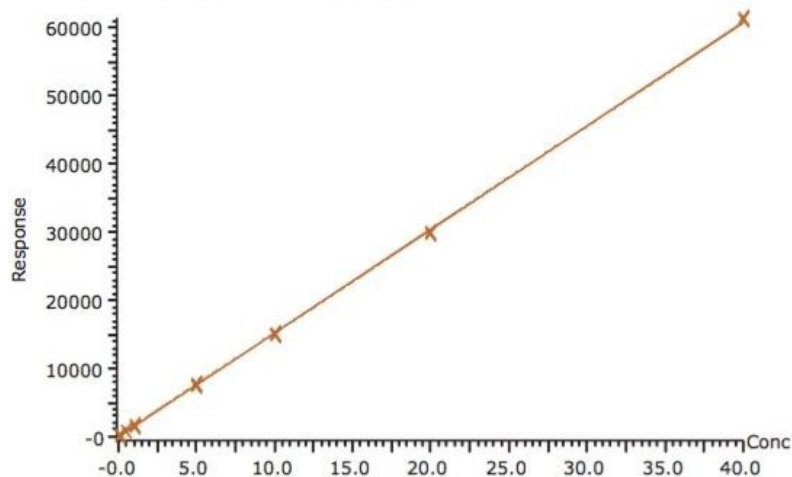

Compound name: Leucomalachite Green
Correlation coefficient: $r = 0.999145$, $r^2 = 0.998292$
Calibration curve: $1.50762 * x + 0.0765038$
Response type: Internal Std (Ref 6), Area * (IS Conc. / IS Area)
Curve type: Linear, Origin: Exclude, Weighting: 1/x, Axis trans: None

60.0

2. European Commission Decision 2002/657/EC of 12 August 2002 implementing Council Directive 96/23/EC concerning the performance of analytical methods and the interpretation of results, as amended by Decision 2003/181/EC(4), (*Official Journal of the European Communities* L 221, 17.08.2002, p. 8–36).
3. Lopez-Gutierrez et al. *Anal Methods*. 5: 3434–3449, 2013.
4. J C Hashimoto et al. *J AOAC Int*. 95: 913–922, 2012.
5. M Kaplan et al. *J Chromatogr A*. 1349: 37–43, 2014.
6. Hurtad-Pessel et al. *J AOAC Int*. 96: 1152–1157, 2013.

Featured Products

[ACQUITY UPLC H-Class PLUS System <https://www.waters.com/10138533>](https://www.waters.com/10138533)

[Xevo TQD Triple Quadrupole Mass Spectrometry <https://www.waters.com/134608730>](https://www.waters.com/134608730)

720005307, February 2015