

ACQUITY UPLC I-Class/Xevo TQD IVD System: Analytical Performance for Catecholamines and Metanephrines

Waters Corporation

这是一份应用简报，不包含详细的实验部分。

供体外诊断使用。仅在部分国家/地区销售。

Abstract

The Waters ACQUITY™ UPLC™ I-Class/Xevo™ TQD IVD System enables the quantification of organic compounds in human biological liquid matrices.

Introduction

The Waters ACQUITY UPLC I-Class/Xevo TQD IVD System enables the quantification of organic compounds in human biological liquid matrices.

This document describes a test of the analytical performance of the ACQUITY UPLC I-Class/Xevo TQD IVD System for the analysis of norepinephrine, epinephrine, dopamine, normetanephrine, metanephrine, and 3-methoxytyramine in urine.



ACQUITY UPLC I-Class/Xevo TQD IVD System.

Experimental

The ACQUITY UPLC I-Class/Xevo TQD IVD System was controlled by MassLynx™ IVD Software (v4.1) and the data processed using the TargetLynx™ Application Manager. Calibrators and Quality Controls were prepared by spiking commercially available reference material in urine and the samples were processed using the following conditions.

Sample Preparation Conditions

400 μ L acidified urine was diluted with 1 mL of 0.5 M ammonium acetate buffer. Samples were loaded onto Oasis™ WCX 30 mg plates, washed, and eluted prior to analysis.

LC Conditions

Column: ACQUITY UPLC BEH Amide 1.7 μ m, 2.1 mm x 100 mm

Mobile phase A:	95:5 Water:acetonitrile containing 50 mM NH ₄ HCOO, pH 3.0
Mobile phase B:	15:85 Water:acetonitrile containing 30 mM NH ₄ HCOO, pH 3.0
Flow rate:	0.6 mL/min
Gradient:	100% B over 1 minute, 100–90% B from 1–2 minutes, 90% B at 1.0 mL/min at 2.1 minutes, 90–70% B from 2.1–2.5 minutes

MS Conditions

Resolution:	MS1 (0.75 FWHM), MS2 (0.75 FWHM)
Acquisition mode:	MRM
Polarity:	ESI (+)

Results and Discussion

Performance characteristics of catecholamines and metanephrines on the ACQUITY UPLC I-Class/Xevo TQD IVD System are shown in Table 1. Analytical selectivity of the chromatographic separation is illustrated in Figure 1.

Compound	Range (ng/mL)	LLOQ (ng/mL)	%RSD at LLOQ	Max imprecision	Max bias
3-methoxytyramine	21.7–521.2	21.7	3.1%	5.0%	9.8%
Metanephrine	11.2–510.7	10.7	1.8%	2.9%	4.0%
Normetanephrine	18.3–517.8	17.8	1.1%	4.2%	3.4%
Epinephrine	0.5–500	0.5	8.6%	6.2%	-4.6%
Dopamine	6.5–506	6.0	4.2%	11%	-7.9%
Norepinephrine	5.1–504.6	4.6	16.3%	14.8%	-6.0%

Table 1. Performance characteristics of the analytes evaluated. Range defined by linear fit where $r^2 > 0.99$. LLOQ defined by $S/N (PtP) > 10$ and $\%RSD \leq 20\%$. $\%RSD$ at LLOQ determined through analytical sensitivity experiments ($n=5$). Maximum imprecision and bias determined over four concentrations ($N=4$).

Note: To convert conventional mass units to SI units multiply by 5.98 for 3-MT, 5.07 for MTN, 5.46 for NMT and EP, 6.53 for DA, and 5.91 for NE. All conversions are from ng/mL to nmol/L.

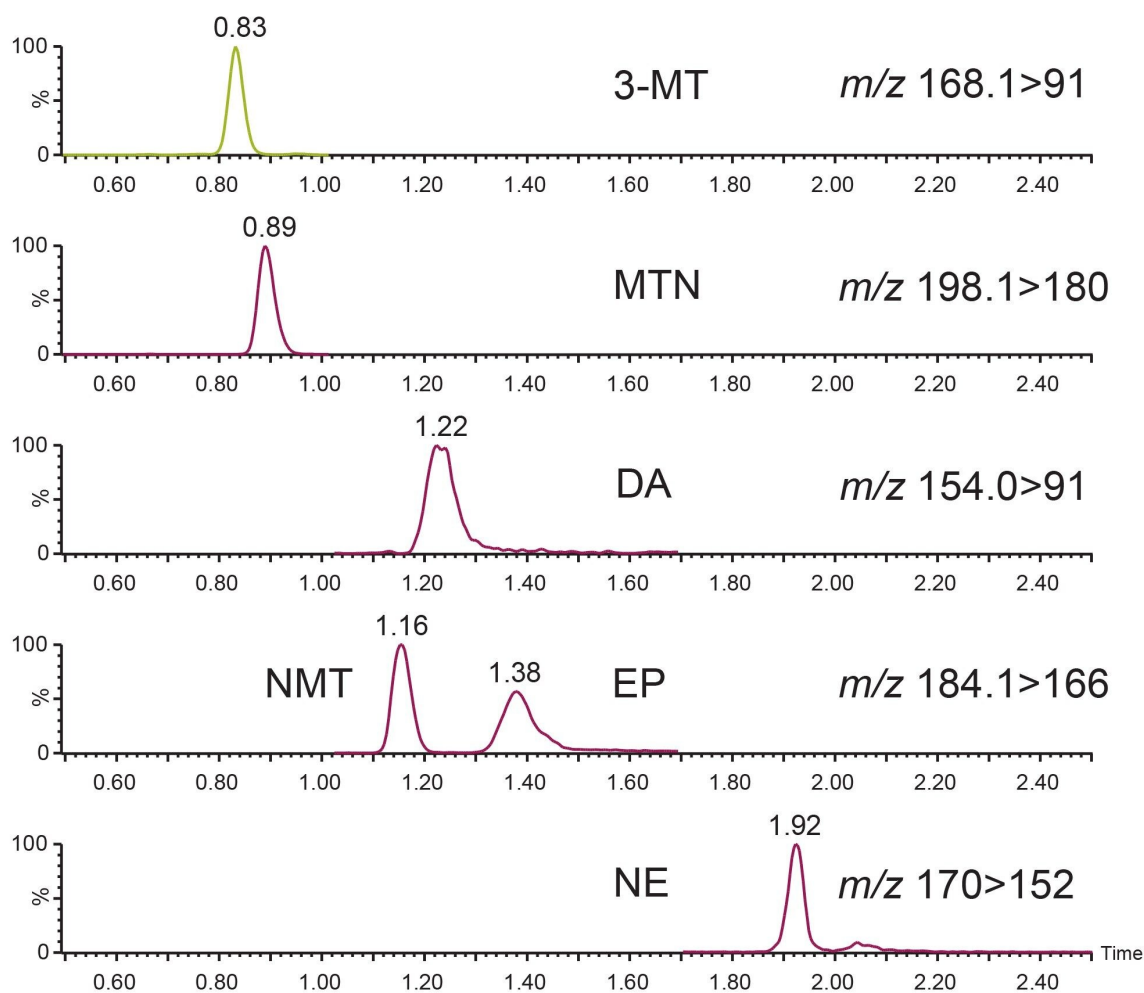


Figure 1. Chromatographic selectivity of catecholamines and metanephrines using the ACQUITY UPLC I-Class/Xevo TQD IVD System.

Note: 3-MT – 3-methoxytyramine; MTN – metanephrine; DA – dopamine; NMT – normetanephrine; EP – epinephrine; NE – norepinephrine.

Conclusion

The Waters™ ACQUITY UPLC I-Class/Xevo TQD IVD System has demonstrated the capability to deliver analytically sensitive and precise chromatography for the analysis of 3-methoxytyramine,

metanephrine, normetanephrine, dopamine, epinephrine, and norepinephrine in urine.

Disclaimer

The analytical performance data presented here is for illustrative purposes only. Waters does not recommend or suggest analysis of the analytes described herein. These data are intended solely to demonstrate the performance capabilities of the system for analytes representative of those commonly analyzed using liquid chromatography and tandem mass spectrometry. Performance in an individual laboratory may differ due to a number of factors, including laboratory methods, materials used, intra-operator technique, and system conditions. This document does not constitute a warranty of merchantability or fitness for any particular purpose, express or implied, including for the testing of the analytes in this analysis.

Featured Products

MassTrak ACQUITY UPLC I-Class PLUS/Xevo TQD IVD System <

<https://www.waters.com/nextgen/global/products/mass-spectrometry-systems/masstrak-acquity-uplc-i-class-plus-xevo-tqd-ivd-system.html>>

MassLynx MS Software <<https://www.waters.com/513662>>

MassLynx Quantitation Applications <<https://www.waters.com/513791>>

720006341, July 2018



© 2024 Waters Corporation. All Rights Reserved.

[使用条款](#) [隐私](#) [商标](#) [招聘](#) [危险化学品生产经营许可证](#) [Cookie](#) [Cookie设置](#)

[沪ICP备06003546号-2](#) [京公网安备 31011502007476号](#)