

Note d'application

Demonstration of LC-MS Nitrosamine Impurity Quantification Performance using Automated Sample Preparation with the Andrew+ Pipetting Robot

Mary Trudeau, Nigel Skinner

Waters Corporation

This is an Application Brief and does not contain a detailed Experimental section.

Want to learn more about the Andrew+ Pipetting Robot?

[REQUEST A DEMO](#)

Abstract

LC-MS analytical method development requires flexible and reproducible sample preparation for accurate and robust analyte quantification. This work highlights automated calibration curve generation using the Andrew+

Pipetting Robot, with cloud-native OneLab Software, for accurate and reproducible LC-MS quantification of nitrosamine impurities, using an ACQUITY UPLC I-Class PLUS System and Xevo TQ-XS Mass Spectrometer.

Benefits

- Accurate, precise, and robust analytic quantification performance
- Ease-of-use and time savings
- Cost savings through increased efficiency and failure reduction
- Less repetitive pipetting
- Automated method transferability

Introduction

Sample preparation is often the most time consuming, but critical, step for the laboratory analyst. Any errors made in the sample preparation step will follow throughout the analysis, potentially causing high variability in performance and in extreme cases failed analysis. In addition, development, optimization, and execution of these assays can prove to be time-consuming and difficult to transfer between scientists and laboratories.¹

Creation of calibration standards and quality control (QC) samples is a requirement in all quantitative analysis. These samples are generated using the basic technique of sequential (or serial) dilution of the analyte(s) from a concentrated solution(s).² While often not difficult, preparation of these samples is repetitive and time-consuming, requiring consistent preparation to ensure the reliable performance of the analytical method. This makes it ideal for incorporating lab automation for this task. It allows the analyst to do other tasks, streamlines the sample preparation process, reduces the potential of human error, and ensures consistent analytical method performance.

The objective of this application brief was to develop an automated sample preparation using the Andrew+ Pipetting Robot for the LC-MS quantification of N-nitrosamine impurities and demonstrate its performance. Due to their carcinogenicity and incidence in a variety of commodities and pharmaceuticals, robust and reliable sample preparation and analysis for their routine quantification during and after drug development and manufacturing is required.

Results and Discussion

The calibration sample preparation protocol was created for the Andrew+ Pipetting Robot based on the sample preparation described in application note p/n: [720006899EN](#) <

<https://www.waters.com/nextgen/us/en/library/application-notes/2020/high-sensitivity-quantitation-of-nitrosamine-genotoxic-impurities-lc-ms-analysis-of-ranitidine-drug-product-using-the-waters-acquity-uplc-i-class-xevo-tq-xs-tandem-quadrupole-mass-spectrometer.html>> . Briefly, three individual calibration curves

containing the six nitrosamine impurities NDMA, NDEA, NEIPA, NDIPA, NDBA, and NMBA were prepared in a water/methanol solution (80/20), water from a concentrated 1 µg/mL stock solution in a 96-well sample

collection plate (p/n: [186005837](#) <<https://www.waters.com/nextgen/us/en/shop/vials-containers--collection-plates/186005837-96-well-sample-collection-plate-700--l-round-well-25-pk.html>>). The reagent preparation

protocol and calibration line protocol were generated in OneLab, the cloud-native software used for both

designing and executing protocols on the Andrew+ Pipetting Robot. This developed protocol not only executes all steps for the calibration line preparation, ranging from 0.025–100 ng/mL, but also provides all the information

for consumables and reagents used during the preparation. Figure 1 highlights the OneLab serial

dilution/calibration curve generation (0.025–100 ng/mL) used in this analysis. Following nitrosamine calibration

curve generation, the analysis plate was sealed with a Silicone/PTFE 96-well cap mat (p/n: [186006332](#) <

<https://www.waters.com/waters/partDetail.htm?partNumber=186006332>>). LC-MS/MS analysis of the

prepared sample was performed using a Waters Xevo TQ-XS Tandem Mass Spectrometer coupled to an

ACQUITY UPLC I-Class PLUS System under MassLynx Software control. Full details of the LC-MS method are

also described in application note p/n: [720006899EN](#) <

<https://www.waters.com/nextgen/us/en/library/application-notes/2020/high-sensitivity-quantitation-of-nitrosamine-genotoxic-impurities-lc-ms-analysis-of-ranitidine-drug-product-using-the-waters-acquity-uplc-i-class-xevo-tq-xs-tandem-quadrupole-mass-spectrometer.html>> .



Figure 1. Andrew+ Pipetting Robot deck layout for serial sample dilution and calibration curve generation.

In accordance with small molecule analytical method development guidance,^{3,4} a developed assay must be able to demonstrate linearity (correlation coefficient or $R^2 \geq 0.98$), accuracy ($\pm 15\%$), and precision ($\pm 15\%$). These criteria were easily achieved for all six (6) N-nitrosamine impurities using the OneLab sample preparation method executed on the Andrew+ Pipetting Robot and subsequent LC-MS analysis. Mean (N=3) calibration performance is demonstrated in Table 1. For all six N-nitrosamine impurities, linear dynamic ranges were 0.025–50 ng/mL, with linear fits ≥ 0.999 using simple 1/x weighting. Additionally, mean accuracy values ranged from 90.7–108.0% with RSDs from 0.2–14.0%, indicating a highly accurate and reproducible method. Representative calibration curves for three of the six nitrosamine impurities are highlighted in Figure 2.

Nitrosamine impurity	Curve (ng/mL)	Weighting	Linear fit (R ²)	Mean % accuracy range	Mean (N=3) % RSD range
NDMA	0.25–50.0	1/X	0.999	94.6–102.1	0.2–4.9
NDEA				95.4–104.6	0.4–8.1
NDBA				92.6–105.3	1.2–4.2
NMBA				96.7–101.8	0.7–14.0
NEIPA				93.0–108.0	0.9–7.5
NDIPA				90.7–105.5	0.7–3.6

Table 1. Nitrosamine impurity LC-MS neat standard quantification performance using Andrew+ Pipetting Robot for serial sample dilution and calibration curve generation.

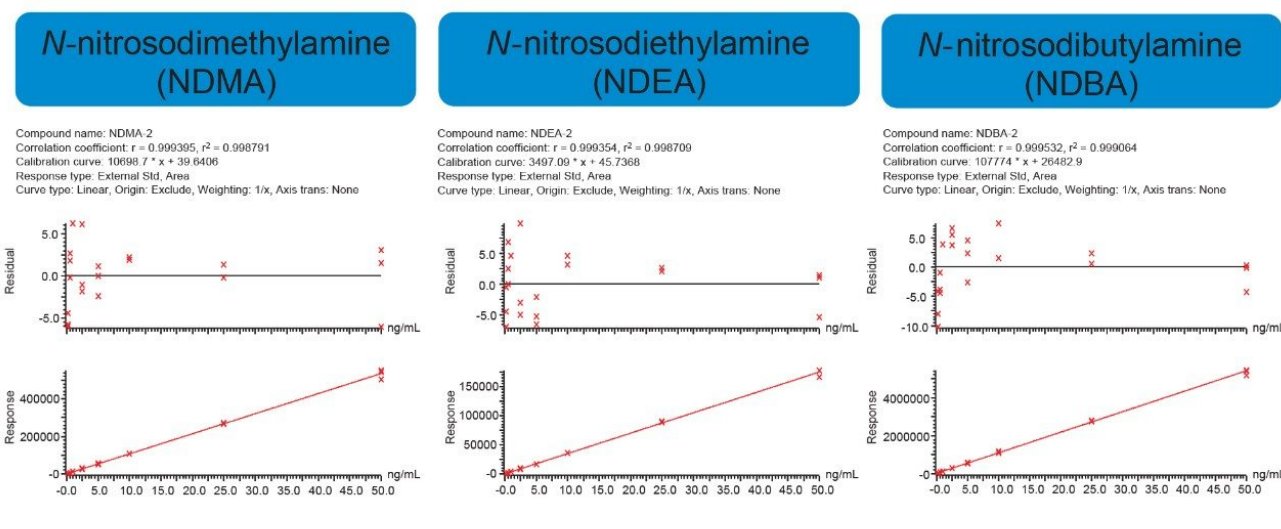


Figure 2. Representative nitrosamine impurity standard calibration curves (NDMA, NDEA, and NDBA) using Andrew+ Pipetting Robot for serial sample dilution and calibration curve generation.

This automated method created with OneLab, and performed on the Andrew+ Pipetting Robot, developed herein, was able to perform simple serial dilution to generate calibration curves for analysis of nitrosamine impurities with no manual intervention by the analyst. This broadly applicable method can be used independently, or as part of a more complex sample workflow for robust LC-MS quantification analysis. In addition, OneLab methods are traceable and easily transferable, ensuring method reproducibility performance: day-to-day, user-

to-user, system-to-system, and lab-to-lab.

References

1. Christler, Anna & Felföldi, Edit & Mosor, Magdalena & Sauer, Dominik & Walch, N. & Dürauer, Astrid & Jungbauer, Alois. (2020). Semi-Automation of Process Analytics Reduces Operator Effect. *Bioprocess and Biosystems Engineering*. 43. 10.1007/s00449-019-02254-y.
2. Accurate and Consistent Serial Dilutions Made Easy with Andrew. Retrieved (22Feb2021) from https://www.andrewalliance.com/wp-content/uploads/2016/10/5_Serial_Dilutions_HD_20161005.pdf <https://www.andrewalliance.com/wp-content/uploads/2016/10/5_Serial_Dilutions_HD_20161005.pdf>
3. Viswanathan, C. T.; Bansal, S.; Booth, B.; DeStefano, A. J.; Rose, M. J.; Sailstad, J.; Shah, V. P.; Skelly, J. P.; Swann, P. G.; Weiner, R. Quantitative Bioanalytical Methods Validation and Implementation: Best Practices for Chromatographic and Ligand Binding Assays. *Pharm. Res.* 2007, 24, 1962–1973.
4. Bansal, S.; DeStefano, A. Key Elements of Bioanalytical Method Validation for Small Molecules. *AAPS J.* 2007, 9, E109–114.

Featured Products

[ACQUITY UPLC I-Class PLUS System <https://www.waters.com/134613317>](https://www.waters.com/134613317)

[Xevo TQ-XS Triple Quadrupole Mass Spectrometry <https://www.waters.com/134889751>](https://www.waters.com/134889751)

[MassLynx MS Software <https://www.waters.com/513662>](https://www.waters.com/513662)

720007134, January 2021



© 2023 Waters Corporation. All Rights Reserved.

[Terms of Use](#) [Privacy](#) [Trademarks](#) [Sitemap](#) [Careers](#) [Cookies](#) [Préférences de cookies](#)