

Note d'application

Enhanced Resolution for Longer Oligonucleotide Analytes With a MaxPeak™ Premier Oligonucleotide BEH C₁₈ 300 Å Column

Balasubrahmanyam Addepalli, Makda Araya, Matthew A. Lauber

Waters Corporation

Abstract

Ion-pairing reversed phase liquid chromatography is widely used to characterize the identity, purity, and integrity of oligonucleotides and this is important to the development and quality control of both diagnostics and therapeutic medicines. Detection sensitivity and retention of these polynucleotide analytes not only depend on the surface chemistry but also pore size of the column stationary phase. The selection of an appropriate pore size can enable longer oligonucleotides to efficiently interact with stationary phase and minimize restricted diffusion effects such that improved peak capacities can be achieved. Here, we report the efficient separation of single stranded (ss) heteromeric deoxyribonucleotide (DNA) ladders on an ACQUITY™ Premier Oligonucleotide BEH C₁₈ 300 Å 1.7 µm Column in a manner that is compatible with online mass spectrometric (MS) detection.

Benefits

- New reference materials for oligonucleotide LC available as ssDNA oligonucleotide ladders
 - Excellent resolution of long-mer oligonucleotides with an ACQUITY Premier Oligonucleotide BEH C₁₈ 300 Å
-

Column

- Improved resolution for oligonucleotides exceeding 70 nucleotides while maintaining performance for shorter oligonucleotides
- Dependable and consistent separation performance independent of the applied ion-pairing reagent
- Reproducible high-quality performance and confident mass measurements

Introduction

Advanced analytical tools are helping to accelerate the development of novel nucleic acid-based diagnostics and therapeutics.¹⁻⁴ Reversed phase liquid chromatography coupled with mass spectrometry (RPLC-MS) is a preferred choice for qualitative and quantitative characterization of the oligonucleotides during various stages of development and pharmacokinetic studies. Volatile alkylamines acting as ion-pairing (IP) reagents improve the retention and resolution of oligonucleotides on reversed phase column during these types of analyses.⁵⁻⁷ The type of IP reagent determines separation selectivity and retention during IP-RPLC.³ Moreover, buffering IP reagents with weak acids like hexafluoroisopropanol makes oligonucleotide IP-RPLC analysis compatible with mass spectrometry (MS).⁸⁻¹⁰

Apart from the surface chemistry of a stationary phase, it is important to consider its pore size. The pore size of a stationary phase can affect the selectivity, retention, and resolution of an oligonucleotide separation. Average pore size determines whether an analyte molecule can diffuse into and out of the porous particle structure and partition between the inter- and intraparticle spaces.¹¹ Smaller pore size (90–130 Å) stationary phases provide larger surface areas per bed length and correspondingly longer retention times for shorter oligonucleotides (<50mer) compared to wider pore size stationary phases (300 Å) with relatively smaller surface area.¹² However, larger analytes encounter steric hindrance when traversing smaller pore structures. This can be seen when analytes are restricted from accessing intraparticle surface areas or show peak broadening from impeding diffusion out of a small pore. In contrast, the wider pore increases the accessibility to longer oligonucleotides and improve the resolution.^{4,12} Here, we present consistently improved resolution and high-quality performance for oligonucleotides above 70mer including 80, 90, and 100mers on a 300 Å pore size premier BEH C₁₈ Column compared to the smaller pore size column.

Experimental

Sample Information

Reference materials were acquired from Waters (Milford, MA). The ssDNA 10 to 60 Ladder (Waters p/n: 186009449 <<https://www.waters.com/nextgen/global/shop/standards--reagents/186009449-ssdna-10-to-60-ladder.html>>) and ssDNA 20 to 100 Ladder (Waters p/n: 186009448 <<https://www.waters.com/nextgen/global/shop/standards--reagents/186009448-ssdna-20-to-100-ladder.html>>) (Table 1) were individually resuspended in 100 µL of Milli-Q water. After gentle mixing, the vial contents were transferred to a 300 µL capacity polypropylene autosampler vial (p/n: 186002639 <<https://www.waters.com/nextgen/global/shop/vials-containers--collection-plates/186002639-polypropylene-12-x-32-mm-screw-neck-vial-with-cap-and-preslit-pt.html>>) for ion-pairing reversed phase liquid chromatography (IP-RP-LC) mass spectrometry (MS) analysis in negative ion mode using the BioAccord™ RDa detector.

Ladder	DNA component	Elemental Composition	Nucleotide Composition	Monoisotopic Mass (Da)	Average Mass (Da)
10 to 60	10mer	C ₉₈ H ₁₂₄ N ₃₇ O ₅₉ P ₉	C:2 T:3 A:2 G:3	3041.544	3043.046
	15mer	C ₁₄₆ H ₁₈₃ N ₆₁ O ₈₈ P ₁₄	C:4 T:2 A:2 G:7	4631.799	4634.059
	20mer	C ₁₉₅ H ₂₄₆ N ₇₅ O ₁₁₈ P ₁₉	C:5 T:5 A:5 G:5	6114.05	6117.045
	25mer	C ₂₄₃ H ₃₀₇ N ₉₃ O ₁₄₈ P ₂₄	C:7 T:6 A:6 G:6	7638.297	7642.032
	30mer	C ₂₉₂ H ₃₆₈ N ₁₁₃ O ₁₇₇ P ₂₉	C:8 T:7 A:8 G:7	9186.555	9191.044
	40mer	C ₃₈₉ H ₄₈₉ N ₁₅₄ O ₂₃₄ P ₃₉	C:11 T:8 A:12 G:9	12268.073	12274.055
20 to 100	50mer	C ₄₈₇ H ₆₁₂ N ₁₉₁ O ₂₉₅ P ₄₉	C:13 T:11 A:14 G:12	15371.573	15379.066
	60mer	C ₅₈₅ H ₇₃₄ N ₂₃₁ O ₃₅₄ P ₅₉	C:15 T:13 A:17 G:15	18484.085	18493.09
	20mer	C ₁₉₅ H ₂₄₆ N ₇₅ O ₁₁₈ P ₁₉	C:5 T:5 A:5 G:5	6114.05	6117.045
	30mer	C ₂₉₂ H ₃₆₈ N ₁₁₃ O ₁₇₇ P ₂₉	C:8 T:7 A:8 G:7	9186.555	9191.044
	40mer	C ₃₈₉ H ₄₈₉ N ₁₅₄ O ₂₃₄ P ₃₉	C:11 T:8 A:12 G:9	12268.073	12274.055
	50mer	C ₄₈₇ H ₆₁₂ N ₁₉₁ O ₂₉₅ P ₄₉	C:13 T:11 A:14 G:12	15371.573	15379.066
	60mer	C ₅₈₅ H ₇₃₄ N ₂₃₁ O ₃₅₄ P ₅₉	C:15 T:13 A:17 G:15	18484.085	18493.09
	70mer	C ₆₈₄ H ₈₅₇ N ₂₇₀ O ₄₁₄ P ₆₉	C:16 T:16 A:20 G:18	21611.596	21622.126
	80mer	C ₇₈₁ H ₉₇₉ N ₃₀₈ O ₄₇₄ P ₇₉	C:19 T:18 A:22 G:21	24700.097	24712.125
	90mer	C ₈₇₈ H ₁₁₀₂ N ₃₄₃ O ₅₃₅ P ₈₉	C:22 T:21 A:24 G:23	27763.591	27777.111
100mer	C ₉₇₆ H ₁₂₂₄ N ₃₈₃ O ₅₉₄ P ₉₉	C:24 T:23 A:27 G:26	30876.103	30891.135	

Table 1. Individual components of the ssDNA 10 to 60 Ladder and the ssDNA 20 to 100 Ladder.

LC Conditions 1

LC system:	ACQUITY Premier BSM System (part of BioAccord System)
Detector:	ACQUITY UPLC TUV Detector
Wavelength:	260 nm
Columns:	ACQUITY Premier Oligonucleotide BEH C ₁₈ , 300 Å, 1.7 µm, 2.1 X 150 mm, p/n: 186010541 ACQUITY Premier Oligonucleotide BEH C ₁₈ , 130 Å, 1.7 µm, 2.1 X 150 mm, p/n: 186009486
Column temperature:	70 °C
Sample temperature:	4 °C
Injection:	5 µL
Flow rate:	0.3 mL/min
Mobile phase A:	7 mM Triethylamine (TEA) as the IP reagent and 40 mM 1,1,1,3,3,3-hexafluoroisopropanol (HFIP) in Milli-Q water, pH 8.6
Mobile phase B:	3.5 mM TEA and 20 mM HFIP in 50:50 Methanol: Milli-Q water

Gradient Table 1

Time (min)	Flow (mL/min)	%A	%B	Curve
Initial	0.3	95	5	*
60.00	0.3	75	25	6
61.00	0.3	50	50	6
62.00	0.3	95	5	6
80.00	0.3	95	5	6
Run time = 80 mins				

LC Conditions 2

LC system:	ACQUITY Premier BSM System (part of BioAccord System)
Detector:	ACQUITY UPLC TUV Detector
Wavelength:	260 nm
Columns:	ACQUITY Premier Oligonucleotide BEH C ₁₈ , 300 Å, 1.7µm, 2.1 X 150 mm ACQUITY Premier Oligonucleotide BEH C ₁₈ , 130 Å, 1.7µm, 2.1 X 150 mm
Column temperature:	70 °C

Sample temperature:	4 °C
Injection:	5 µL
Flow rate:	0.4 mL/min
Mobile phase A:	0.1% N,N-diisopropylethylamine (DIPEA) as the IP reagent and 1% 1,1,1,3,3,3-hexafluoroisopropanol (HFIP) in Milli-Q water
Mobile phase B:	0.0375% DIPEA and 0.075% HFIP in 65:35 Acetonitrile: Milli-Q water

Gradient Table 2

Time (min)	Flow (mL/min)	%A	%B	Curve
Initial	0.4	95	5	*
60.00	0.4	82	18	6
60.50	0.4	5	95	6
61.00	0.4	95	5	6
80.00	0.4	95	5	6
Run time = 80 mins				

MS Conditions

MS system:	BioAccord LC-MS System
Detector:	ACQUITY RDa Detector
Mode:	Full scan with fragmentation
Polarity:	Negative
Cone voltage:	40 V
Fragmentation cone voltage:	80–200 V
Mass range:	High (400–5000 <i>m/z</i>)
Scan rate:	2 Hz
Capillary voltage:	0.80 kV
Desolvation temperature:	400 °C

Informatics

The Intact Mass analysis application of the waters_connect™ platform was employed to compute the neutral mass values of oligonucleotides.

Results and Discussion

The ssDNA 10 to 60 and 20 to 100 Ladders were analyzed by IP-RP-LC-MS using a set of ACQUITY Premier Oligonucleotide BEH C₁₈ Columns containing 300 Å or 130 Å pore size sorbents. Data were acquired in triplicate in negative ion mode, where the cone voltage of electrospray source was alternated between low energy (40 V) and high energy (80–200 V) to acquire the mass values of intact and fragmented oligonucleotides.

Improved resolution of oligonucleotide analytes using a 300 Å pore size BEH C₁₈ sorbent is illustrated in Figures 1–2. Figure 1 shows an overlay of the LC-UV chromatograms obtained with both the ladders using a triethylamine (TEA)-HFIP mobile phase system. Although these columns with different pore size sorbents exhibit similar chromatographic resolution up to 60mer, the wide pore 300 Å column exhibited marked improvement of the separation for 70, 80, 90, and 100mers compared to 130 Å pore size column. The latter column resolved 70 and 80mer as one set of peaks compared to the 90 and 100mer peak set, where the individual components of the pair are only partially resolved. However, both columns yielded the expected number of oligonucleotide peaks, eight for 10 to 60 ladder and nine for 20 to 100 ladder. Importantly, the resolution of shorter oligonucleotides is also maintained without any compromise due to the use of the wider pore column. Interestingly, the identical oligonucleotide standards (20, 30, 40, 50, and 60mer) present in both ladders exhibited near identical retention times even though each ladder was injected independently. This type of reproducible behavior is highly suited to the detection of identical analyte/s in multiple samples, as is encountered in oligonucleotide therapeutic development, DMPK studies and bioanalysis. The oligonucleotide component observed in each chromatographic peak was confirmed by the acquired electrospray MS spectra (data not shown). As predicted, the 130 Å pore size column produced longer retention times compared to wider pore sorbent column, presumably due to higher pore surface area as proposed in other studies.¹²

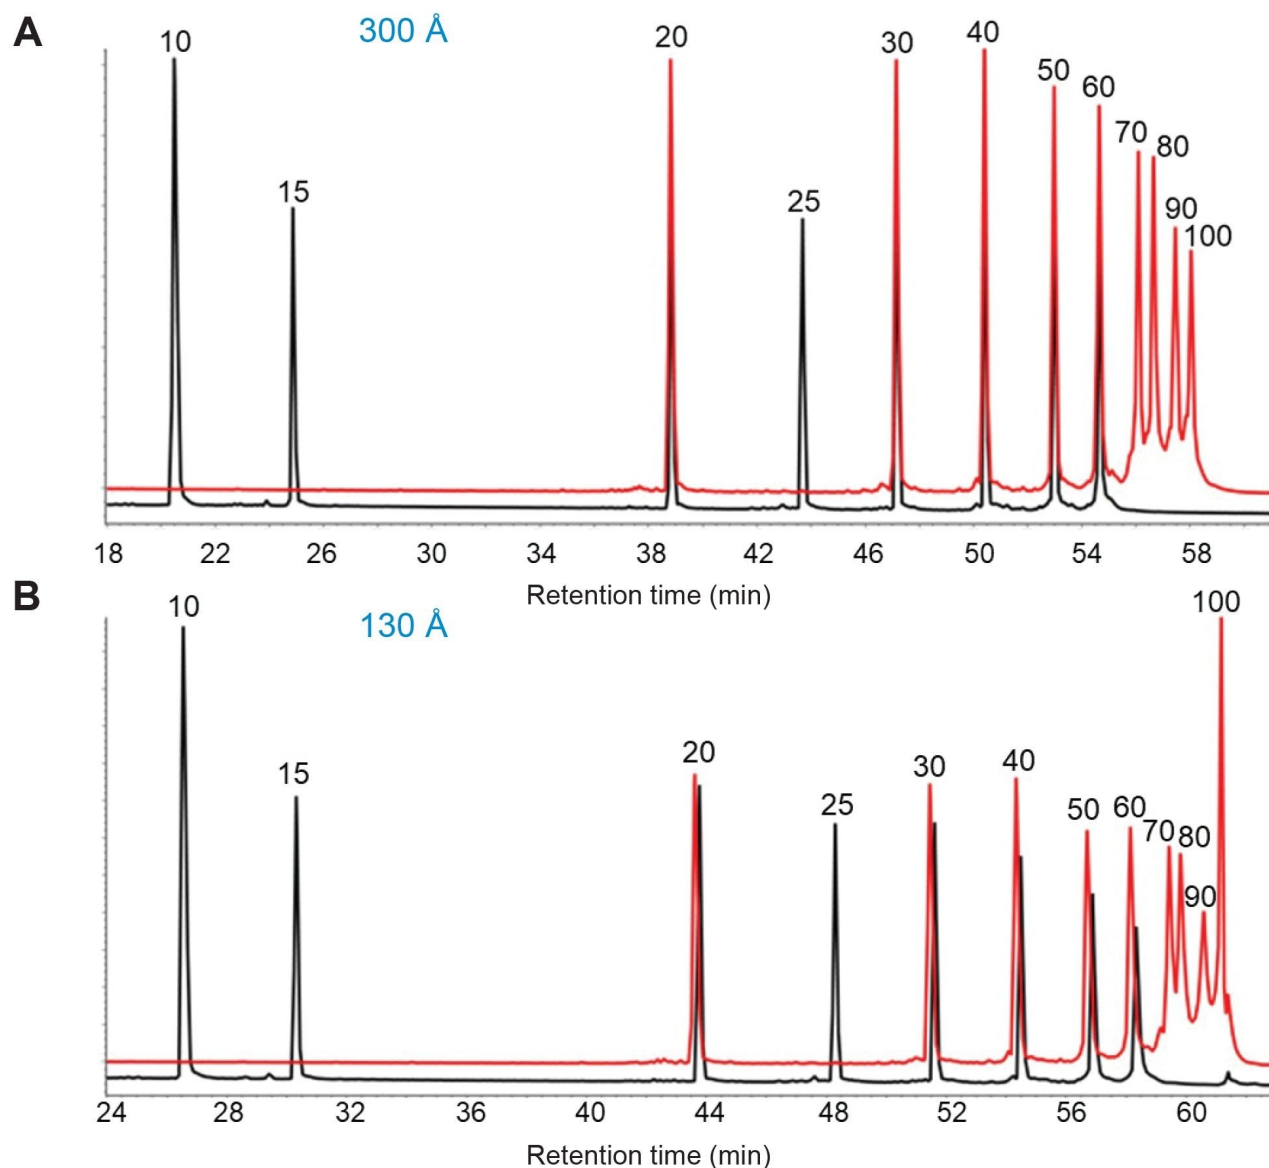


Figure 1. Comparative separation of single stranded DNA oligonucleotide ladders (black trace: 10–60, red trace: 20–100 ladder) on an ACQUITY Premier BEH C_{18} Column with 300 Å (A) and 130 Å (B) pore sizes. IP-RPLC-UV chromatograms of oligonucleotide ladders obtained with a TEA-HFIP mobile phase system are shown. Peaks are annotated by their corresponding nucleotide lengths.

Figure 2 depicts the chromatographic profiles of 10 to 60mer and 20 to 100mer ladders following IP-RP-LC-MS on the 300 Å pore size column using a diisopropylethylamine (DIPEA)-HFIP mobile phase. This mobile phase

system exhibited slightly improved resolution for 70, 80, 90, and 100mer DNA ladder components. This indicates robust separation performance for more than one mobile phase system. The slightly enhanced chromatographic resolution that came with the use of DIPEA made it possible to achieve even higher quality MS data.¹³

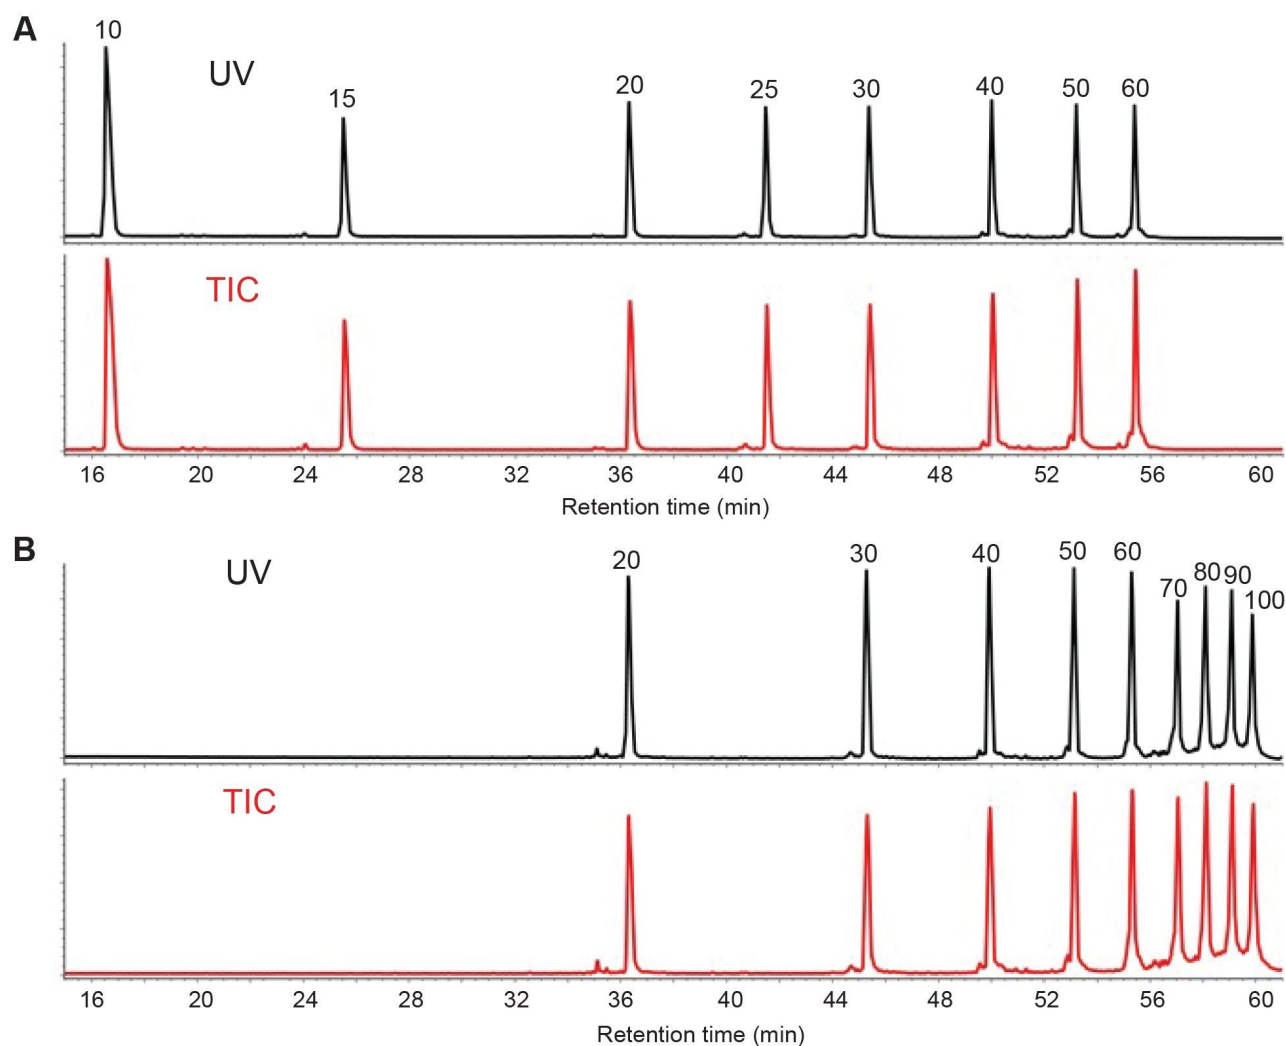


Figure 2. IP-RPLC-UV-MS chromatograms of oligonucleotide ladders (A: ssDNA 10 to 60 Ladder, B: 20 to 100 Ladder) obtained by using an ACQUITY Premier Oligonucleotide BEH C₁₈ 300 Å 1.7 µm Column and DIPEA-HFIP mobile phase system. UV trace is denoted by black and TIC by red trace. Peaks are annotated by their corresponding nucleotide lengths.

The mass measurements of the resolved oligonucleotide peaks are illustrated in Figure 3 and Table 2. Figure 3

shows the electrospray ion series of the mass spectra obtained for the chromatographic peaks corresponding to 90 (59.12 min, MW 27,778) and 100mer (59.90 min, MW 30,892) ssDNA ladder components. Intact mass analysis of each spectra revealed neutral mass values that correspond well (mass error of <60 ppm) with the expected average mass values.

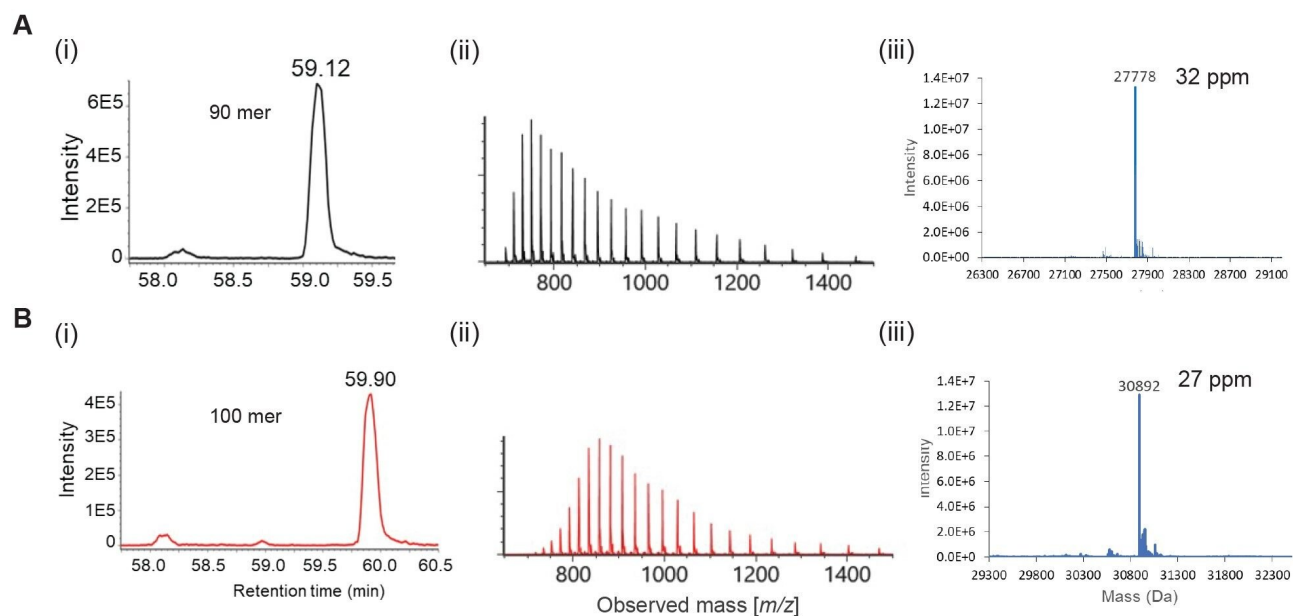


Figure 3. Intact mass analysis of the LC-MS spectra of 90 (A) and 100mer (B) oligonucleotide components from the ssDNA 20 to 100 Ladder. The electrospray series of multiply charged ions were deconvoluted using the Intact Mass application of waters_connect to get the neutral mass values. The chromatographic peak (i), mass spectrum (ii) and the deconvoluted mass values (iii) are shown. Mass error is indicated in ppm.

Sample	DNA component	Monoisotopic mass (Da)	Average mass (Da)	Experimental intact mass (Da)	Mass error (ppm)
10–60 Ladder	10 mer	3041.544	3043.046	3041.666	40
	15 mer	4631.799	4634.059	4631.959	35
	20 mer	6114.05	6117.045	6114.403	58
	25 mer	7638.297	7642.032	7638.717	55
	30 mer	9186.555	9191.044	9186.353	-22
	40 mer	12268.073	12274.06	12268.370	24
	50 mer	15371.573	15379.07	15380.000	60
	60 mer	18484.085	18493.09	18494.000	49
20–100 Ladder	20 mer	6114.05	6117.045	6114.354	50
	30 mer	9186.555	9191.044	9186.353	-22
	40 mer	12268.073	12274.06	12268.370	24
	50 mer	15371.573	15379.07	15380.000	60
	60 mer	18484.085	18493.09	18494.000	49
	70 mer	21611.596	21622.13	21623.000	40
	80 mer	24700.097	24712.13	24713.000	35
	90 mer	27763.591	27777.11	27778.000	32
	100 mer	30876.103	30891.14	30892.000	28

Table 2. Deconvoluted mass values of the electrospray ion series of the mass spectra obtained with the ACQUITY Premier Oligonucleotide BEH C₁₈ 300 Å 1.7 µm Column using a DIPEA-HFIP mobile phase system. The neutral mass values produced by the Intact Mass application of the waters_connect platform were compared against either monoisotopic mass (light blue shade) or average mass (light green) of the oligonucleotides to compute the mass error in ppm.

Table 2 depicts the intact mass values of the individual oligonucleotides following deconvolution of the mass spectra by the Intact Mass application of the waters_connect platform. Examination of these deconvoluted mass values indicated higher propensity to match with the monoisotopic mass for oligonucleotides up to 40mer (MW 12,268) and average mass at above 50mer DNA (MW 15,380). This observation confirms that the BioAccord LC-MS System and its RDa mass spectrometer tends to produce a mass resolution of approximately 10,000.

Finally, UV detector response was assessed and found to be highly reproducible when examined from three independent injections of each ladder where the RSD values were <3% (Figure 4).

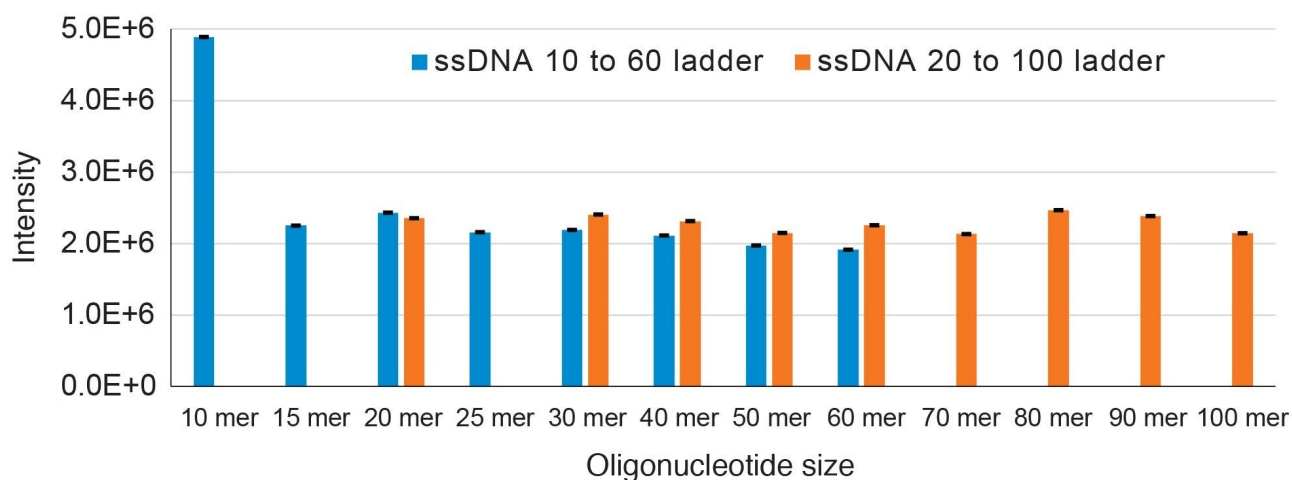


Figure 4. Reproducible TUV detector response of the individual oligonucleotides from three injections of each ladder. Blue bars denote the response of components from the ssDNA 10 to 60 Ladder and orange bars indicate the same from the ssDNA 20 to 100 Ladder. The RSD of detector response stayed <3% for all measurements.

Conclusion

The ACQUITY Premier Oligonucleotide BEH C₁₈, 300 Å Column provides improved resolution for longer oligonucleotide analytes while maintaining excellent resolution of shorter oligonucleotides. The availability of two new LC-Certified reference materials made it possible to quickly confirm the suitability of this type of column with two different ion pairing mobile phase systems. Oligonucleotides of the same size and nucleotide composition exhibited identical retention times irrespective of the sample origin, indicating that these methods are highly suitable for peak tracking and peak ID applications. Ultimately, the combination of high peak capacity column described here and the compliance ready BioAccord LC-MS System has made it significantly easier to achieve in depth analyses of oligonucleotides (and potentially beyond) of 100 nucleotides in length.

References

1. Goyon, A., P. Yehl, and K. Zhang, Characterization of Therapeutic Oligonucleotides by Liquid Chromatography. *Journal of Pharmaceutical and Biomedical Analysis*, 2020. 182: p. 113105.
2. Demelenne, A., *et al.*, Analytical Techniques Currently Used in the Pharmaceutical Industry for the Quality Control of RNA-Based Therapeutics and Ongoing Developments. *Journal of Chromatography A*, 2021. 1651: p. 462283.
3. Donegan, M., J.M. Nguyen, and M. Gilar, Effect of Ion-Pairing Reagent Hydrophobicity on Liquid Chromatography and Mass Spectrometry Analysis of Oligonucleotides. *Journal of Chromatography A*, 2022. 1666: p. 462860.
4. Fornstedt, T. and M. Enmark, Separation of Therapeutic Oligonucleotides Using Ion-Pair Reversed-Phase Chromatography Based on Fundamental Separation Science. *Journal of Chromatography Open*, 2023. 3: p. 100079.
5. Apffel, A., *et al.*, New Procedure for the Use of High-Performance Liquid Chromatography–Electrospray Ionization Mass Spectrometry for the Analysis of Nucleotides and Oligonucleotides. *Journal of Chromatography A*, 1997. 777(1): p. 3–21.
6. Gilar, M., *et al.*, Ion-Pair Reversed-Phase High-Performance Liquid Chromatography Analysis of Oligonucleotides: Retention Prediction. *Journal of Chromatography A*, 2002. 958(1): p. 167–182.
7. Huber, C.G., P.J. Oefner, and G.K. Bonn, High-Resolution Liquid Chromatography of Oligonucleotides on Nonporous Alkylated Styrene-Divinylbenzene Copolymers. *Analytical Biochemistry*, 1993. 212(2): p. 351–358.
8. Martin Gilar, K.J.F., Yeva Budman, Jeffrey L. Holyoke, Hamid Davoudi, and John C. Gebler, Characterization of Therapeutic Oligonucleotides Using Liquid Chromatography With On-Line Mass Spectrometry Detection. *Oligonucleotides*, 2003. 13(4): p. 229–243.
9. Erb, R. and H. Oberacher, Comparison of Mobile-Phase Systems Commonly Applied in Liquid Chromatography-Mass Spectrometry of Nucleic Acids. *ELECTROPHORESIS*, 2014. 35(9): p. 1226–1235.
10. McGinnis, A.C., E.C. Grubb, and M.G. Bartlett, Systematic Optimization of Ion-Pairing Agents and Hexafluoroisopropanol for Enhanced Electrospray Ionization Mass Spectrometry of Oligonucleotides. *Rapid Communications in Mass Spectrometry*, 2013. 27(23): p. 2655–2664.
11. Wang, Y., *et al.*, A Theoretical Study of the Separation Principle in Size Exclusion Chromatography.

Macromolecules, 2010. 43(3): p. 1651–1659.

12. Bagge, J., *et al.*, Impact of Stationary-Phase Pore Size on Chromatographic Performance Using Oligonucleotide Separation as a Model. *Journal of Chromatography A*, 2020. 1634: p. 461653.
13. Croley, T.R., *et al.*, The Chromatographic Role in High Resolution Mass Spectrometry for Non-targeted Analysis. *Journal of The American Society for Mass Spectrometry*, 2012. 23(9): p. 1569–1578.

Featured Products

BioAccord LC-MS System for Biopharmaceuticals <<https://www.waters.com/waters/nav.htm?cid=135005818>>

ACQUITY Premier System <<https://www.waters.com/waters/nav.htm?cid=135077739>>

ACQUITY UPLC Tunable UV Detector <<https://www.waters.com/514228>>

ACQUITY RDa Detector <<https://www.waters.com/waters/nav.htm?cid=135077027>>

720007926, May 2023

© 2023 Waters Corporation. All Rights Reserved.

[Conditions d'utilisation](#) [Confidentialité](#) [Marques](#) [Carrières](#) [Cookies](#) [Préférences de cookies](#)